



Technology for Vacuum Systems

# VACUUM PUMP

VACUU·PURE 10



## Instructions for use



## **Original instructions Keep for further use!**

*This manual is only to be used and distributed in its complete and original form. It is strictly the user's responsibility to carefully check the validity of this manual with respect to the product.*

Manufacturer:

**VACUUBRAND GMBH + CO KG**  
**Alfred-Zippe-Str. 4**  
**97877 Wertheim**  
**GERMANY**

Phone:

Head office +49 9342 808-0  
Sales +49 9342 808-5550  
Service +49 9342 808-5660

Fax: +49 9342 808-5555

Email: [info@vacuubrand.com](mailto:info@vacuubrand.com)

Web: [www.vacuubrand.com](http://www.vacuubrand.com)

*Thank you for purchasing this product from **VACUUBRAND GMBH + CO KG**. You have chosen a modern and technically high quality product.*

## TABLE OF CONTENTS

<b>1</b>	<b>Introduction</b>	<b>5</b>
1.1	User information . . . . .	5
1.2	About this document. . . . .	6
1.2.1	Manual structure . . . . .	6
1.2.2	Display conventions . . . . .	7
1.2.3	Symbols and icons . . . . .	8
1.2.4	Handling instructions (action steps). . . . .	9
1.2.5	Abbreviations . . . . .	10
1.2.6	Term definitions. . . . .	10
<b>2</b>	<b>Safety information</b>	<b>13</b>
2.1	Usage . . . . .	13
2.1.1	Intended use . . . . .	13
2.1.2	Improper use. . . . .	14
2.1.3	Foreseeable misuse. . . . .	14
2.2	Obligations . . . . .	15
2.2.1	Operator obligations . . . . .	15
2.2.2	Personnel obligations . . . . .	15
2.3	Target group description. . . . .	16
2.4	General safety information . . . . .	17
2.4.1	Safety precautions . . . . .	17
2.4.2	Protective clothing. . . . .	17
2.4.3	Laboratory and working materials. . . . .	18
2.4.4	Chemical compatibility of materials. . . . .	18
2.4.5	Eliminate sources of danger . . . . .	19
2.5	Motor protection . . . . .	23
2.6	Disposal . . . . .	23
<b>3</b>	<b>Product description</b>	<b>24</b>
3.1	VACUU·PURE 10 . . . . .	26
3.2	Optional accessories . . . . .	27
3.2.1	Vacuum pump accessories. . . . .	27
3.2.2	VACUU·BUS accessories . . . . .	29
3.2.3	Modbus RTU protocol. . . . .	30
<b>4</b>	<b>Installation and connection</b>	<b>31</b>
4.1	Transport . . . . .	31
4.2	Set up the vacuum pump . . . . .	32
4.3	Connection . . . . .	34
4.3.1	Vacuum connection (IN) . . . . .	34
4.3.2	Outlet connection (OUT). . . . .	38
4.3.3	Electrical connection. . . . .	41

<b>5</b>	<b>Commissioning (operation)</b>	<b>42</b>
5.1	Switch on . . . . .	42
5.2	Operation . . . . .	42
5.2.1	Operation . . . . .	44
5.2.2	Regeneration mode . . . . .	45
5.2.3	Autostart . . . . .	46
5.3	Advanced operation . . . . .	47
5.3.1	Display of software / hardware version . . . . .	47
5.3.2	Restore factory settings . . . . .	49
5.3.3	Remote operation via Modbus RTU . . . . .	50
5.4	Connect / remove VACUU·BUS accessories . . . . .	51
5.4.1	VACUU·BUS detection . . . . .	52
5.4.2	Operation with VACUU·BUS accessories . . . . .	53
5.5	Shutdown (switch off) . . . . .	54
5.6	Storage . . . . .	55
<b>6</b>	<b>Error messages</b>	<b>56</b>
6.1	Warning display . . . . .	56
6.2	Error indication . . . . .	57
6.3	Troubleshooting . . . . .	58
6.3.1	Technical support . . . . .	58
6.3.2	Error – Cause – Remedy . . . . .	59
<b>7</b>	<b>Cleaning and maintenance</b>	<b>65</b>
7.1	Information on maintenance work . . . . .	66
7.2	Cleaning . . . . .	67
7.2.1	Clean the vacuum pump . . . . .	67
7.3	Air inlet filter . . . . .	68
7.4	Replace the device fuse . . . . .	69
<b>8</b>	<b>Appendix</b>	<b>70</b>
8.1	Technical information . . . . .	70
8.1.1	Technical data . . . . .	70
8.1.2	Rating plates . . . . .	74
8.1.3	Wetted materials . . . . .	75
8.2	Ordering information . . . . .	76
8.3	Service . . . . .	78
8.4	Index . . . . .	79
8.5	EC Declaration of conformity . . . . .	81

# 1 Introduction

This manual is part of your product. The manual applies to all versions of the vacuum pump and is intended in particular for laboratory staff.

## 1.1 User information

### Safety

---

Instructions for use  
and safety

- Read this manual thoroughly and completely before using the product.
- Keep this manual in an easily accessible location.
- Correct use of the product is essential for safe operation. Comply with all safety information provided!
- In addition to this manual, adhere to the accident prevention regulations and industrial safety regulations applicable in the country of use.

### General

---

General  
information

- For easier readability, the general term *vacuum pump* is used as an equivalent to and instead of the product name *Vacuum Pump VACUU·PURE 10*.
- If passing the product on to a third party, also give them this manual.
- The illustrations in this manual are only intended to facilitate comprehension.
- We reserve the right to make technical changes in the course of continuous product improvement.

### Copyright

---

Copyright © and  
copyright law

The content of this manual is protected by copyright. Only copies for internal use are allowed, e.g., for professional training.

© VACUUBRAND GMBH + CO KG

**Contact**

Contact us

- If your manual is incomplete, you can request a replacement. Alternatively, you can use our download portal: [www.vacuubrand.com](http://www.vacuubrand.com)
- You are welcome to contact us at any time in writing or by telephone if you would like more information, have questions about our products or wish to share feedback with us.
- When contacting our Service Department, please have the serial number and product type at hand → *see Rating plates on the product.*

**1.2 About this document**


**1.2.1 Manual structure**

Specific information

The manual has a modular structure with separate instruction modules for the vacuum pump and any accessories.

**Instruction modules**

Vacuum pump and modular instruction manuals

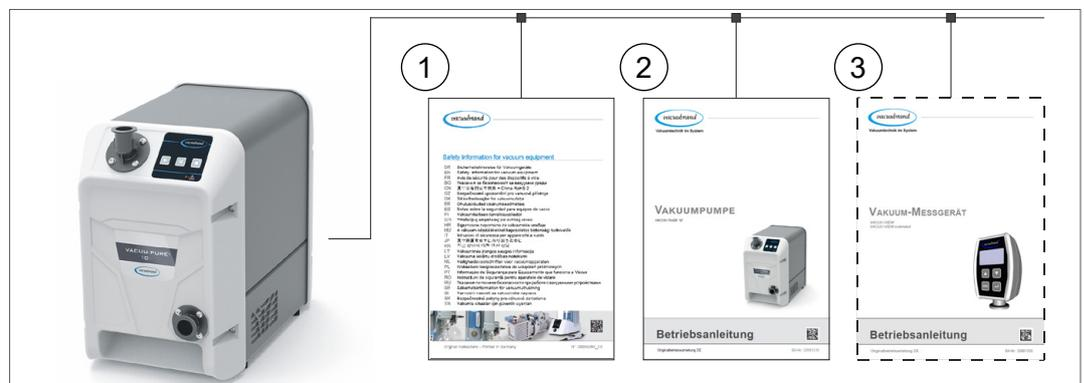

Description

- 1** Safety information for vacuum equipment
- 2** Description: Vacuum pump – connection, operation, service
- 3** Optional description: Accessories

## 1.2.2 Display conventions

### Warning levels

Display conventions

	<b>DANGER</b>
	<p><b>Warns of an imminent hazard.</b></p> <p>Disregarding the situation could result in extremely serious injury or death.</p> <p>⇒ Take appropriate action to avoid dangerous situations!</p>

	<b>WARNING</b>
	<p><b>Warns of a potentially hazardous situation.</b></p> <p>Disregarding the situation could result in serious injury or death.</p> <p>⇒ Take appropriate action to avoid dangerous situations!</p>

	<b>CAUTION</b>
	<p><b>Indicates a potentially hazardous situation.</b></p> <p>Disregarding the situation could result in minor injury or damage to property.</p> <p>⇒ Take appropriate action to avoid dangerous situations!</p>

<b>NOTE</b>
<p><b>Indicates a potentially harmful situation.</b></p> <p>Disregarding the situation could result in damage to property.</p>

### Additional notes

**IMPORTANT!**

- ⇒ Information or specific recommendation which must be observed.
- ⇒ Important information for trouble-free operation of your product.

	<ul style="list-style-type: none"> <li>⇒ Helpful tips + tricks</li> <li>⇒ Additional information</li> </ul>
---	---

### 1.2.3 Symbols and icons

This manual uses symbols and icons. Safety symbols indicate specific risks associated with handling the product. Symbols and icons are designed to help you identify risks more easily.

#### Safety symbols


Explanation of safety symbols

	Hazardous substance – hazards to human health.		General prohibition sign.
	General warning symbol.		Warning: risk of explosion.
	Danger: electricity.		Warning: hot surface.
	General mandatory sign.		Disconnect power plug.

#### Additional symbols and icons

Additional symbols

	Positive example – <b>Do this!</b> Result – OK		Negative example – <b>Don't do this!</b>
	<b>Press key</b>		<b>Keep key pressed</b>
	Refers to content in this manual.		Refers to content in other supplementary documents.

 Electric/electronic devices must not be disposed of in domestic waste at the end of their service life.

 Installation at temperatures < 40 °C.

 Ensure sufficient air circulation.

 Flow arrow, inlet – vacuum connection

 Flow arrow, outlet

### 1.2.4 Handling instructions (action steps)

#### Instructions (single step)

Action steps as text ⇒ Perform the step described.

- Result of action


#### Instructions (multiple steps)

1. First step
2. Next step


- Result of action

#### Instructions (shown graphically)

Schematic diagram  
Action steps as  
graphics

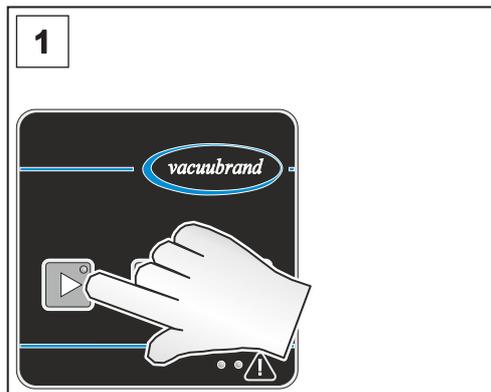

1. First step

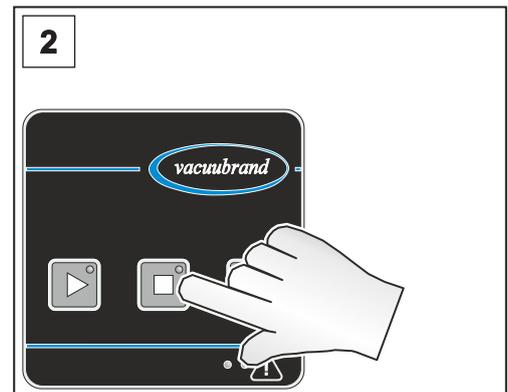

2. Next step

- Result of action

⇒ Perform the steps in the order described.

### 1.2.5 Abbreviations

#### Abbreviations

<b>abs.</b>	Absolute
<b>ATM</b>	Atmospheric pressure
<b>d<sub>i</sub></b> (di)	Interior diameter
<b>DN</b>	Nominal diameter
<b>FKM</b>	Fluoroelastomer
<b>IN</b>	Inlet, vacuum connection
<b>KF</b>	Small flange
<b>max.</b>	Maximum
<b>min</b>	Minutes
<b>OUT</b>	Outlet
<b>PBT</b>	Polybutylene terephthalate
<b>PEEK</b>	Polyetheretherketone
<b>PPS</b>	Polyphenylene sulfide
<b>PTFE</b>	Polytetrafluoroethylene
<b>PVF</b>	Polyvinyl fluoride
<b>RMA no.</b>	Return Merchandise Authorization number
<b>RTU</b>	Remote Terminal Unit
<b>Resp.</b>	Responsible

### 1.2.6 Term definitions

#### Product-specific terms

<b>Autostart</b>	When the power supply is switched off and then back on, the last active operating state of the vacuum pump is automatically reactivated.
<b>Fine vacuum</b>	Pressure range in vacuum technology, from: 1 mbar – 0.001 mbar (0.75 Torr – 0.00075 Torr)
<b>Rough vacuum</b>	Pressure range in vacuum technology, from: atmospheric pressure – 1 mbar (atmospheric pressure – 0.75 Torr)
<b>Modbus RTU</b>	Communication protocol for communication with the vacuum pump. ▶ See separate manual for description of the Modbus RTU.
<b>Regeneration mode</b>	Operating mode of the vacuum pump, when the pump unit is dried by ambient air sucked in at reduced pump speed.
<b>Check valve (internal)</b>	Internal valve for safe operation of the vacuum pump. No vacuum-tight switch-off when the vacuum pump stops.

<b>VACUU·BUS</b>	Bus system from <b>VACUUBRAND</b> for communication between peripheral devices and VACUU·BUS-enabled products.
<b>VACUU·BUS address</b>	Address which enables the VACUU·BUS client to be unambiguously assigned within the bus system, e.g., for connecting multiple sensors with the same measuring range.
<b>VACUU·BUS client</b>	Peripheral device or component with VACUU·BUS port, which is integrated in the bus system, e.g., sensors, valves, etc.
<b>VACUU·BUS configuration</b>	Assigning a different VACUU·BUS address to a VACUU·BUS component using a gauge or controller.
<b>VACUU·BUS connector</b>	4-pin round connector for the bus system from <b>VACUUBRAND</b> .
<b>VACUU·PURE Shuttle</b>	Mobile base frame for the vacuum pump.
<b>VACUU·VIEW extended</b>	External vacuum sensor with VACUU·BUS port, 1100 – 0.001 mbar. ▶ for connection to the vacuum pump or with own plug-in power supply.



## 2 Safety information

The information in this chapter must be observed by everyone who works with the product described here.

The safety information is valid for the entire life cycle of the product.

### 2.1 Usage

Only use the product if it is in perfect working condition.

#### 2.1.1 Intended use

Intended use The **VACUU·PURE 10** is a compact, oil-free, air-cooled vacuum pump for the rough and fine vacuum range in the laboratory for pumping non-corrosive gases. The vacuum pump may only be used indoors in a dry, non-explosive atmosphere.

#### Intended use also includes:



- observing the information in the document **Safety information for vacuum equipment**,
- observing the manual,
- observing the manual of connected components,
- regularly inspecting the vacuum pump according to its operating conditions and have this carried out by qualified personnel,
- using only approved accessories or spare parts.

Any other use is considered improper use.

## 2.1.2 Improper use

Improper use Incorrect use or any application which does not correspond to the technical data may result in injury or damage to property.

### Improper use includes:

- using the product contrary to its intended use,
- using the product in non-commercial environments, unless the necessary protective measures and precautions have been taken by the company,
- operation under inadmissible environmental and operating conditions,
- operation despite obvious errors or defective safety devices,
- unauthorized extensions, conversions, or repairs, in particular when these impair safety,
- the use of unauthorized accessories or spare parts,
- usage despite incomplete assembly,
- operation by insufficiently trained or qualified personnel,
- switching on/off with tools or one's foot,
- operation with sharp-edged objects,
- pulling plug-in connections on the cable out of the socket,
- extracting or conveying solids or liquids.

## 2.1.3 Foreseeable misuse

Misuse In addition to improper use, there are types of use which are prohibited when handling the product:



### Prohibited types of use include, in particular:

- use on humans or animals,
- installation and operation in potentially explosive atmospheres,
- use in mines or underground,
- unauthorized modifications,
- switching on/off with tools or one's foot,
- operation with sharp-edged objects,
- using the product to generate pressure,
- fully exposing the product to the vacuum, immersing it in liquids, exposing it to water spray or steam jets,

- Misuse
- pumping corrosive gases,
  - pumping oxidizing and pyrophoric substances, liquids or solids,
  - pumping hot, unstable, or explosive media,
  - pumping substances which may react explosively under impact and/or elevated temperature without an air supply.

**IMPORTANT!**

**No foreign bodies, hot gases or flames from the application must be allowed to enter the equipment.**

→ see chapter: 8.1.1 Technical data on page 70.

## 2.2 Obligations

### 2.2.1 Operator obligations

Operator obligations

The owner defines the responsibilities and ensures that only trained personnel or specialists work on the product. This applies in particular to connection work and troubleshooting.

Users must have the appropriate qualifications for the listed activities; see *Responsibility matrix*. In particular work on electrical equipment must be performed only by qualified electricians.

### 2.2.2 Personnel obligations

Personnel obligations

If the product is not in proper working order, it must be prevented from being accidentally switched back on.

- ⇒ Always be conscious of safety and work in a safe manner.
- ⇒ Observe instructions issued by the operator, and national regulations on accident prevention and industrial safety.



The way individuals act can help to prevent accidents at work.

## 2.3 Target group description

Target groups The manual must be read and observed by every person who is tasked with the activities described below.

### Personnel qualification

Qualification description

<b>Operator</b>	Laboratory staff, such as chemists, laboratory technicians
<b>Specialist</b>	Person with professional qualification in mechanics, electrical equipment or laboratory devices
<b>Responsible specialist</b>	Specialist with additional specialist, departmental or area responsibility

### Responsibility matrix

Responsibility matrix

Activity	Operator	Specialist	Responsible specialist
Transport	x	x	x
Installation	x	x	x
Commissioning	x	x	x
Operation	x	x	x
Updates			x
Error report	x	x	x
Remedy	(x)	x	x
Repair order			x
External cleaning	x	x	x
Clean the filter at the air intake and fan grilles	x	x	x
Shutdown		x	x
Decontamination <sup>1</sup>		x	x

<sup>1</sup> Alternatively, arrange for decontamination by a qualified service provider

## 2.4 General safety information

Quality standards  
and safety

Products from **VACUUBRAND GMBH + CO KG** are subject to stringent quality testing with regard to safety and operation. Each product undergoes a comprehensive test program prior to delivery.

⇒ Observe the instructions for all actions as specified in this manual.

### 2.4.1 Safety precautions

Safety precautions

⇒ Use your product only if you have understood its function and this manual.

⇒ Replace defective parts immediately, e.g., a broken power cord or faulty hoses.

⇒ Use only original accessories and components designed for vacuum technology, such as a vacuum hose, vacuum valve, etc.

⇒ When handling contaminated parts, follow the relevant regulations and protective measures; this also applies to equipment sent in for repair.

---

**Prior to returning any product to our Service Department for repair, contamination from hazardous substances needs to be excluded.**


**IMPORTANT!**

⇒ Therefore, send us the carefully completed and signed [Health and Safety Clearance](#) certificate before sending your product for repair.

---

### 2.4.2 Protective clothing

Protective clothing



No special protective clothing is required to operate the vacuum pump. Observe instructions issued by the operator for your workplace.

**IMPORTANT!**

⇒ When handling chemicals, wear your personal protective equipment.

---

### 2.4.3 Laboratory and working materials

	<b>DANGER</b>
<p><b>Hazardous substances could be discharged at the outlet.</b></p> <p>During aspiration, hazardous, toxic substances at the outlet can get into the ambient air.</p> <ul style="list-style-type: none"> <li>⇒ Observe the relevant safety regulations for safe handling of hazardous substances.</li> <li>⇒ Please note that residual process media may pose a danger to people and the environment.</li> <li>⇒ Mount and use suitable separators, filters or fume hood devices.</li> </ul>	

- ⇒ Prevent the release of hazardous, toxic, explosive, corrosive fluids, gases or vapors or those that are harmful to health or the environment, for example, through suitable laboratory facilities with a fume hood and ventilation control.

#### Hazards due to different substances

Pumping different substances

Pumping different substances or media can cause the substances to react with one another.

- ⇒ Be aware of interactions and possible chemical reactions of the pumped media.
- ⇒ Dry the vacuum pump with ambient air before changing the medium to be pumped. Use regeneration mode of the vacuum pump for this purpose  
→ *see chapter: 5.2.2 Regeneration mode on page 45.*

### 2.4.4 Chemical compatibility of materials

Compatibility of the vacuum pump with pumped substances

Working materials which get into the vacuum pump with the gas flow can damage the vacuum pump. Substances can be deposited in the vacuum pump.

- ⇒ Check the compatibility of the pumped substances with the wetted materials of the vacuum pump  
→ *see chapter: 8.1.3 Wetted materials on page 75.*
- ⇒ Contact us if you have concerns about using your vacuum pump with certain working materials or media.

## 2.4.5 Eliminate sources of danger

### Connect the tubing correctly

Avoid overpressure

No inadmissible pressure must be created at the vacuum pump outlet. If the back pressure at the outlet is inadmissibly high, pumped media may escape → see *chapter: 8.1.1 Technical data on page 70*.

- ⇒ Always ensure that the outlet line is clear and has no back pressure. The outlet must not be blocked, to ensure that gases can exit freely.
- ⇒ Prevent uncontrolled overpressure (e.g., due to a locked or blocked piping system, condensate, or clogged outlet line).
- ⇒ At the gas connections, the connections for the inlet and outlet must not be mixed up. The inlet is indicated by a directional arrow on the connecting flange.
- ⇒ Observe the maximum pressures at the inlet and outlet of the vacuum pump, as specified in *chapter 8.1.1 Technical data on page 70*.
- ⇒ The system to be evacuated as well as all hose connections must be mechanically stable.
- ⇒ Attach hoses to optional hose nozzles (e.g., adapters at pump connections) so that they do not come loose unintentionally.

### Danger when using regeneration mode

Regeneration mode

During regeneration mode, ambient air passes through the pump unit. Pumped media can form reactive mixtures with ambient air.

- ⇒ Make sure that the pumped media combined with air never leads to reactive, explosive, or otherwise dangerous mixtures.

## **Prevent condensate return**

Condensate in the outlet line

Condensate in the outlet line can damage the vacuum pump. Condensate must not flow back into the outlet or vacuum pump through the hose line. Liquid must not accumulate inside the outlet line.

⇒ Preferably route the outlet line with a fall from the outlet, i.e., running downward so that no backup forms.

## **Prevent foreign bodies inside the pump**

Foreign bodies

Particles and dust must not enter the vacuum pump during normal operation.

⇒ Do not pump any substances which could form deposits inside the vacuum pump.

⇒ Install suitable filters upstream of the inlet. Suitable filters are chemically resistant, clog-proof and have a reliable flow rate, for example.

⇒ Replace porous vacuum hoses without delay.

## **Hazards during venting**

Hazards during venting

The vacuum pump does not create a vacuum-tight seal when it switches off. Depending on the application, venting can cause explosive mixtures to form in systems or other hazardous situations to arise.

⇒ Install a shut-off valve in the inlet line to isolate your application from the vacuum pump with a vacuum-tight seal.

Hazards due to automatic restart of the vacuum pump (Autostart)

### Dangers due to vacuum pump Autostart

The vacuum pump has an Autostart function. When the power supply is switched off and then back on, the last active operating state of the vacuum pump is automatically reactivated, e.g.:

- after a power failure,
- after switching the vacuum pump off and on,
- after disconnecting and reconnecting the power plug.

An ongoing process starts automatically when the power supply is disconnected and reconnected.

- ⇒ Check whether this function can be used safely with the planned application.
- ⇒ Ensure that the automatic restart of the process does not pose any danger to persons or equipment.
- ⇒ Take appropriate safety precautions (e.g., shut-off valve, relay switch, protection against restart) if an automatic restart of the vacuum pump can lead to a dangerous situation.
- ⇒ The Autostart function can be deactivated via Modbus RTU protocol; see separate manual for Modbus RTU description.

Hazards due to residual energy

### Hazards due to residual energy

After the vacuum pump has been switched off and disconnected from the power supply, there may still be dangers due to residual energy:

- Thermal energy: motor waste heat, compression heat.
- ⇒ Let the vacuum pump cool down before carrying out maintenance work.

## Hazards due to overheating

Overheating The vacuum pump can be damaged due to overheating. Possible causes include insufficient air supply to the fan, failure to maintain minimum distances, ambient temperature outside the specified operating conditions. Overheating of the vacuum pump can lead to a reduction in the speed of the vacuum pump or to the vacuum pump being switched off.

- ⇒ When installing the product, ensure that there is a minimum distance of 5 cm between the vacuum pump and adjacent parts (such as the housing, walls, etc.).
- ⇒ Always ensure that there is a sufficient air supply and air extraction to remove the warm exhaust air from the vacuum pump, especially if the vacuum pump is installed in a housing or lab furniture. Provide external forced ventilation.
- ⇒ Place the product on a stable surface. A soft surface such as foam rubber can impair and block the air supply.
- ⇒ Clean polluted ventilation slots.
- ⇒ Avoid excessive heat input due to hot process gases.
- ⇒ Observe the maximum admissible media temperature  
→ *see chapter: 8.1.1 Technical data on page 70.*
- ⇒ Allow the vacuum pump to cool down before servicing or cleaning.

## Keep signs legible

Labels and signs Keep any signs affixed to the product in an easily readable condition:

- ⇒ Labels
- ⇒ Warning and information signs
- ⇒ Rating plates

## 2.5 Motor protection

Overheating protection, blockage protection

The pump motor has a temperature sensor on the circuit board as overload protection. In the event of excessive temperature or if the motor is blocked, the vacuum pump switches off.

If the vacuum pump is switched off due to these safety precautions, the error must be cleared manually: Unplug vacuum pump from power supply → eliminate cause of error → switch vacuum pump back on.

## 2.6 Disposal

### NOTE

**Electronic devices must not be disposed of in domestic waste at the end of their service life.**

Used electronic devices contain harmful substances that can cause damage to the environment or human health. Disused electrical devices also contain valuable raw materials, which can be recovered for reuse if the device is disposed of correctly within the recycling process.

End users are legally obliged to take used electric and electronic devices to a licensed collection point.

Correctly dispose of all electronic scrap and electronic components at the end of their service life.

⇒ Observe the national regulations regarding disposal and environmental protection.



### 3 Product description

Product description The **VACUU·PURE 10** is an oil-free, air-cooled screw vacuum pump for the vacuum range from atmospheric pressure to  $10^{-3}$  mbar in the laboratory for pumping non-corrosive gases.

VACUU·BUS system As a component of the VACUU·BUS system, the vacuum pump offers numerous connection and expansion options for a wide variety of applications.

#### Product features

Technical characteristics

- The operating principle of the vacuum pump is based on the non-contact gap seal.
- The suction chamber of the vacuum pump is oil-free.
- The vacuum pump also offers a high pumping speed for light gases.
- An internal non-return valve protects the vacuum pump against faulty start-up. A vacuum-tight shutdown can be achieved by an additional external valve.




#### Condensate compatibility

Compatible with water vapor and condensate

Due to the high level of water vapor and condensate compatibility of the vacuum pump, no gas ballast is required. Condensate or drops of liquid that enter the vacuum pump with the pumped medium are easily conveyed through the vacuum pump.

## Drying function

Regeneration mode




The vacuum pump has an integrated regeneration mode for drying the inside of the pump after the application is finished or before it is taken out of service.


- During regeneration mode, ambient air is fed into the interior of the pump and the interior is dried by the air supply.
- The vacuum pump can remain connected to the process during regeneration.
- During regeneration, the vacuum pump runs at reduced speed.

### 3.1 VACUU-PURE 10

Side and front view

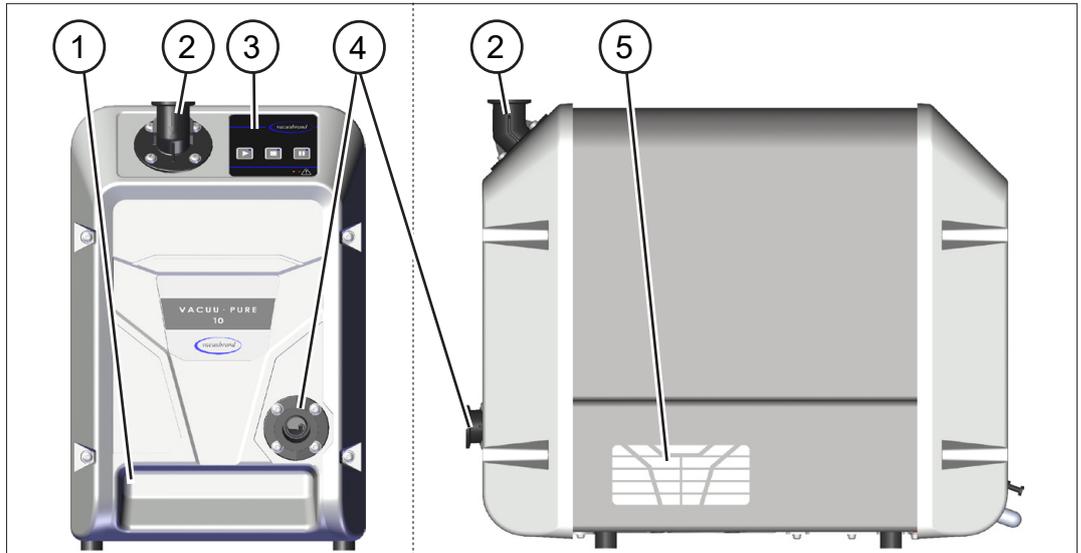

Rear view

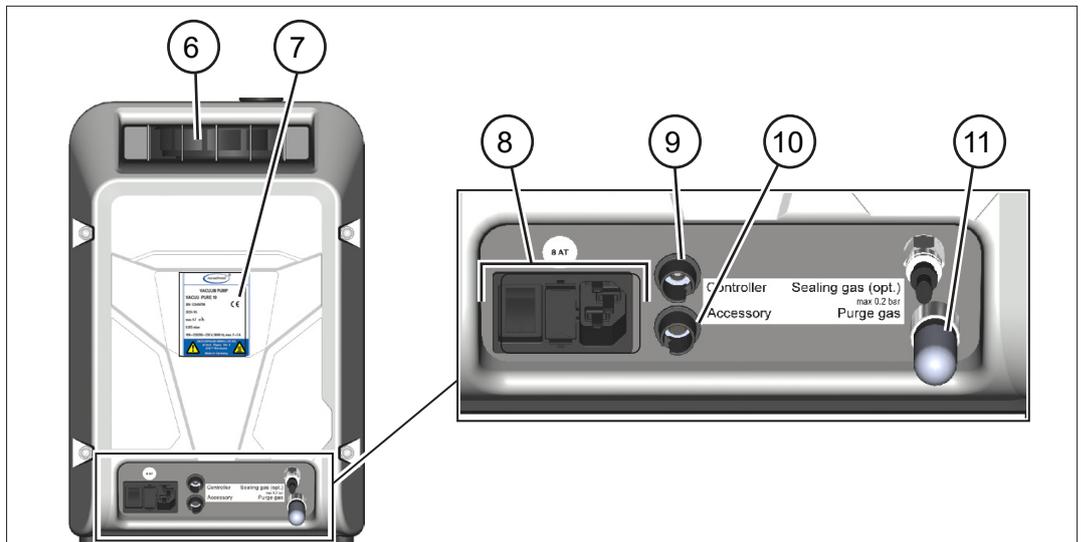

Description

- |    |  |
|----|--|
| 1  | Recessed grip on front                                 |
| 2  | Inlet – vacuum connection                              |
| 3  | Control panel  |
| 4  | Outlet – outlet connection                             |
| 5  | Air vents  |
| 6  | Recessed grip on rear + cooling air outlet             |
| 7  | Rating plate   |
| 8  | Power connection, device fuse, on/off switch           |
| 9  | VACUU-BUS plug-in connection / Modbus connection       |
| 10 | VACUU-BUS socket: Accessories                          |
| 11 | Air filter for ambient air supply in regeneration mode |

## 3.2 Optional accessories

→ see also chapter: 8.2 Ordering information on page 76.

### 3.2.1 Vacuum pump accessories

Optional accessories for the vacuum pump

A silencer and the **VACUU·PURE Shuttle** are available as separate accessories for mounting on the vacuum pump.

#### Silencer

The silencer reduces noise at the pump outlet and, if required, can be attached directly to the outlet flange by means of a small flange connection KF DN 25.

- The silencer must only be used when pumping dry gases.
- When pumping vapors it is mandatory to connect an outlet line instead.


#### VACUU·PURE Shuttle

The shuttle facilitates the movement of the vacuum pump.

The vacuum pump is mounted directly on the shuttle.

## Overview of vacuum pump accessories

Optional  
accessories:  
Silencer and  
VACUU·PURE  
Shuttle

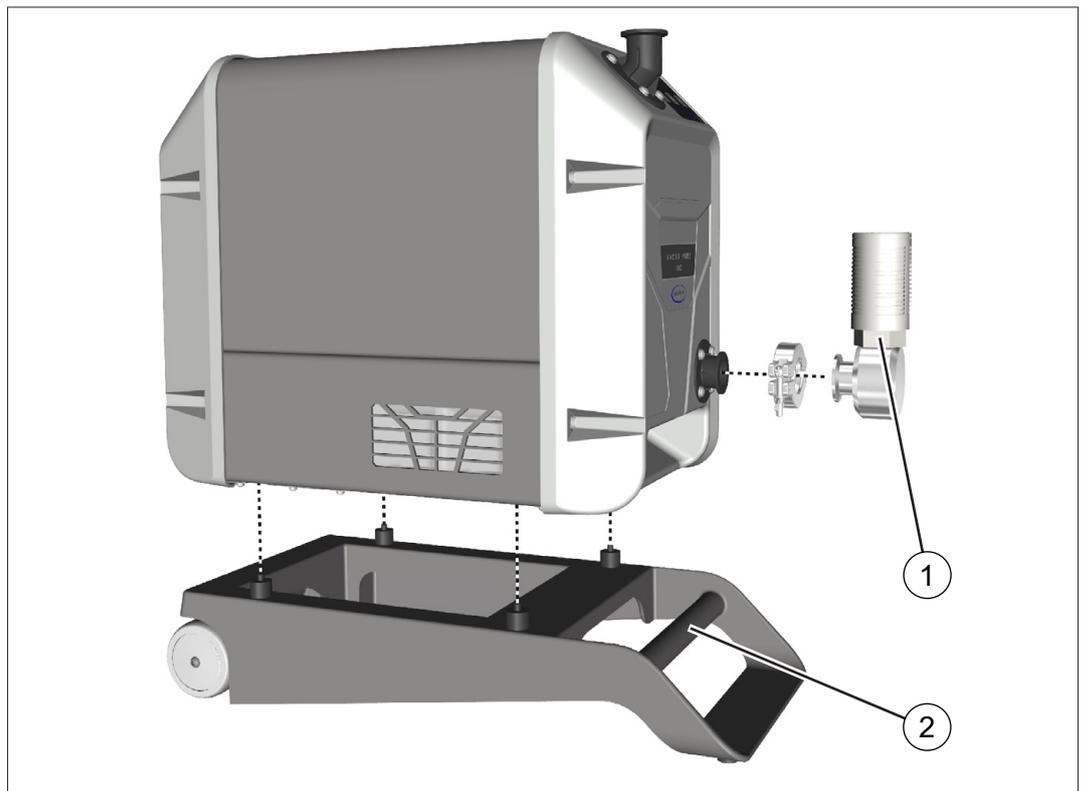

- 1 Silencer at the outlet of the vacuum pump; connection via KF DN 25
- 2 **VACUU·PURE Shuttle**

**3.2.2 VACUU·BUS accessories**

Connect VACUU·BUS components

The lower VACUU·BUS port on the back of the vacuum pump offers a variety of expansion options for connecting VACUU·BUS components.

You can use VACUU·BUS extension cables and Y adapters to distribute and connect several components.

The maximum permissible total power at the VACUU·BUS socket is 11 W.

**Overview of VACUU·BUS accessories**

→ Examples VACUU·BUS components



Description

1 Vacuum gauge VACUU·VIEW extended 1100 – 0.001 mbar	1.3 W
2 In-line solenoid valve VV-B 15C	9.5 W


→ see also chapter: 8.2 Ordering information on page 76.

### 3.2.3 Modbus RTU protocol

The upper VACUU·BUS port on the back of the vacuum pump is intended for remote operation of the vacuum pump, via Modbus RTU protocol → *see separate manual for description of the Modbus RTU.*

#### Connection Modbus RTU

→ Examples  
Modbus RTU

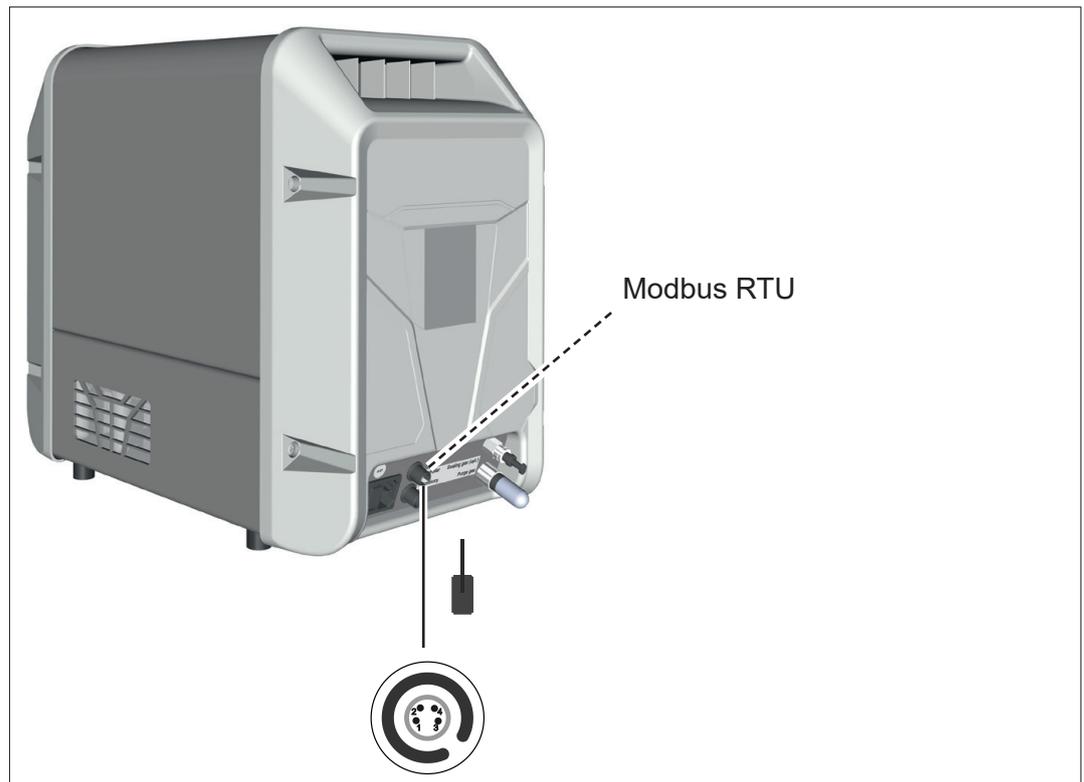

## 4 Installation and connection

### 4.1 Transport

Products from **VACUUBRAND** are packed in sturdy, recyclable packaging.



The original packaging is accurately matched to your product for safe transport.

If possible, please keep the original packaging, e.g., for returning the product for repair.


### Goods receipt

Check the shipment for transport damage and completeness.

⇒ Immediately report any transport damage in writing to the supplier.

### Unpacking

→ Example  
Vacuum pump in  
original packaging

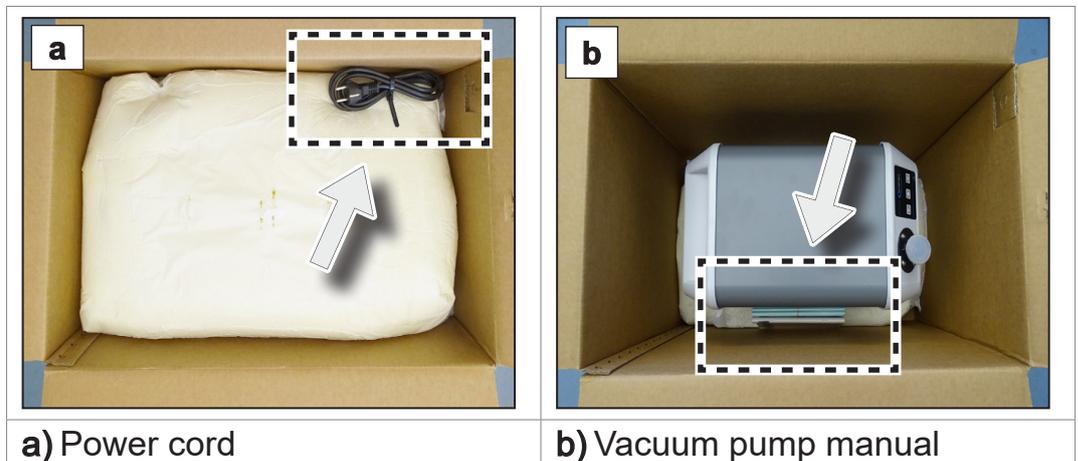

⇒ Remove the upper part of the foam packaging.



- ⇒ Note that the **weight of the vacuum pump is approx. 21 kg.**
- ⇒ Carefully lift the vacuum pump out of the packaging using the recessed grips.

## 4.2 Set up the vacuum pump

### NOTE

#### **Condensate can damage the electronics.**

A large temperature difference between the storage location and the installation location can cause condensation.

- ⇒ After goods receipt or storage, allow your product to acclimatize before initial use. Acclimatization can take several hours.


### Check installation conditions

Check installation conditions

- The product is acclimatized.
- The ambient conditions are within the limitation of use → see *chapter: Observe limitation of use on page 33.*
- The vacuum pump must have a stable and secure base without additional mechanical contact apart from the pump feet.

**Set up the vacuum pump**

→ Example  
Sketch of minimum  
distances in lab  
furniture

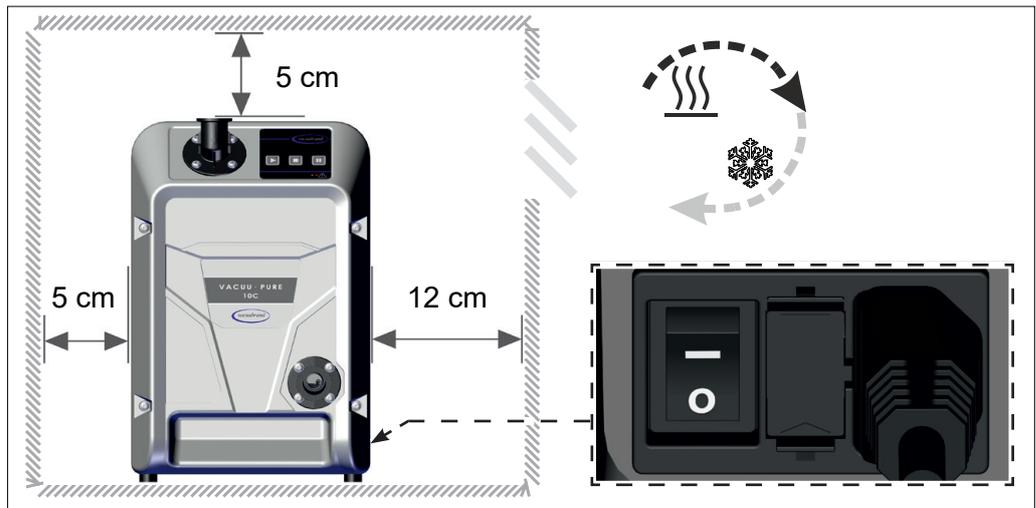

⇒ Place the vacuum pump on a stable, non-vibrating, level surface.

**IMPORTANT!**

⇒ When installing in lab furniture, maintain a minimum distance of 5 cm (2 in) to adjacent objects or surfaces.

⇒ The product must be positioned so that the on/off switch and the power plug can be reached and are accessible, minimum distance 12 cm (5 in).

⇒ Prevent heat accumulation and ensure sufficient air circulation, especially in closed housings.

⇒ Always ensure that there is an adequate air supply and air extraction to remove the warm exhaust air from the vacuum pump. Provide external forced ventilation with a volume flow of approx. 100 m<sup>3</sup>/h when installing in lab furniture.

**Observe limitation of use**

Observe limitation  
of use

Limitation of use	(US)	
Operating ambient temperature	10 – 40 °C	50 – 104 °F
Max. altitude	2000 m above sea level	6562 ft above sea level
Minimum distance to adjacent parts	5 cm (12 cm)	2 in (5 in)
Relative humidity	30 – 85 %, non-condensing	
Pollution degree	2	
Protection class	IP 20	NEMA type 1
Prevent condensation or external contamination from dust, liquids, and corrosive gases.		

**IMPORTANT!**

- ⇒ Note the IP protection class. IP protection is only guaranteed if the product is appropriately mounted and connected.
- ⇒ When connecting, observe the information on the rating plate and chapter **8.1.1 Technical data on page 70**.


**4.3 Connection**

The vacuum pumps have a vacuum connection and an outlet connection. Connect your vacuum pump as described in the examples below.

**4.3.1 Vacuum connection (IN)**

Vacuum connection (IN)

The vacuum connection is indicated by a directional arrow on the inlet connector.

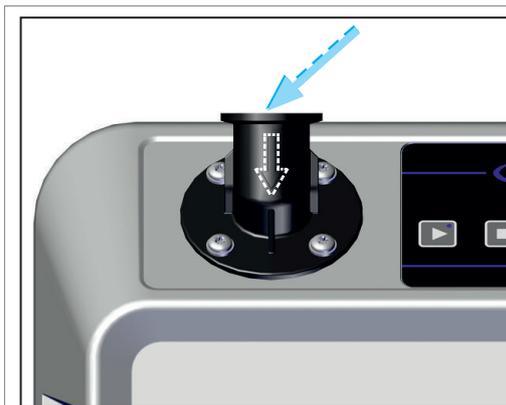

Vacuum connection

	<b>CAUTION</b>
	<p><b>Flexible vacuum hoses can contract during evacuation.</b></p> <p>Connected components that are not secured can cause injury or damage due to the jerky movement (shrinkage) of a flexible vacuum hose. The vacuum hose can come loose.</p> <ul style="list-style-type: none"> <li>⇒ Secure the vacuum hose to the connections.</li> <li>⇒ Secure connected components.</li> <li>⇒ Take the maximum shrinkage into account when sizing the flexible vacuum hose.</li> </ul>

**NOTE**

**Foreign bodies in the inlet line can damage the vacuum pump.**

⇒ Prevent particles and contaminants from being aspirated or being able to flow back.

**IMPORTANT!**

- ⇒ Use a sufficiently stable vacuum hose that is designed for the required vacuum range.
- ⇒ Keep the vacuum hose as short as possible.
- ⇒ Connect a vacuum hose with as large a cross-section as possible.
- ⇒ The connection between vacuum hose and the vacuum pump must be gas-tight.
- ⇒ Avoid kinks in the vacuum hose.

## Rotate the inlet flange

The inlet flange can be rotated in 90° increments.


→ Example  
Rotate inlet flange  
forward



1. Loosen the 4 screws on the inlet flange: Torx screwdriver TX25, paying attention to the washers.



2. Remove the inlet flange. Check the O-ring for damage and that it is correctly seated.

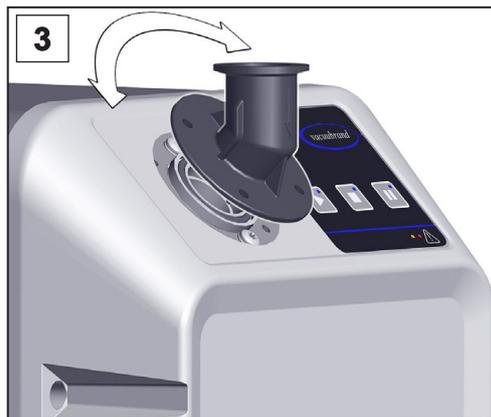

3. Turn the inlet flange in the required direction.



4. Screw on the inlet flange together with the washers; Torx screwdriver TX25.

### Connect the vacuum hose

Vacuum hose at the inlet

- ⇒ Connect a vacuum hose with small flange KF DN 25 to the inlet flange, ensuring the connection is gas-tight.
- ⇒ Alternatively, you can use an adapter from small flange KF DN 25 on the hose nozzle and attach a vacuum hose to it. Secure hose connections on hose nozzles, e.g., with a hose clip.
- ⇒ If necessary, install an in-line solenoid valve or shut-off valve in the inlet line to isolate your application from the vacuum pump with a vacuum-tight seal.



Observe the following points for optimum results:

- ⇒ Keep the vacuum line as short as you can with as large a cross-section as possible.

### 4.3.2 Outlet connection (OUT)

Connect the outlet line to the outlet

	<b>WARNING</b>
	<p><b>Risk of bursting due to overpressure inside the outlet line.</b></p> <p>Inadmissibly high pressure in the outlet line can cause the vacuum pump to burst or damage seals.</p> <ul style="list-style-type: none"><li>⇒ The outlet line (exhaust gas, gas outlet) must always be clear and non-pressurized.</li><li>⇒ Always route the outlet line with a fall or take measures to prevent condensate from flowing back into the vacuum pump.</li><li>⇒ Observe the maximum admissible pressures and pressure differences.</li></ul>

	<b>CAUTION</b>
	<p><b>Excess pressure at the outlet can cause pumped media to escape.</b></p> <p>If the outlet is blocked, pumped media can escape from the vacuum pump and cause personal injury and/or pump damage.</p> <ul style="list-style-type: none"><li>⇒ Do not block the outlet. Do not kink the outlet line.</li><li>⇒ Do not install a shut-off valve in the outlet line.</li><li>⇒ Use an outlet line with a sufficient cross-section.</li></ul>

## Connect the outlet line

Outlet line at the outlet

- ⇒ Connect an outlet line with small flange KF DN 25 to the outlet flange, ensuring the connection is gas-tight.
- ⇒ Alternatively, you can use an adapter from small flange KF DN 25 on the hose nozzle and attach the outlet line to it. Use an outlet line with an interior diameter of at least 19 mm → see *chapter: 8.2 Ordering information on page 76*. Secure hose connections on hose nozzles, e.g., with a hose clip.
- ⇒ Route the outlet line with a fall from the outlet, i.e., running downward so that no backup forms.
- ⇒ The length of the outlet line must not exceed 5 m. An excessively long outlet line can lead to inadmissibly high back pressure at the outlet.

**IMPORTANT!**

## Connect the silencer (option)

Silencer at the outlet

	<b>WARNING</b>
	<p><b>Risk of bursting due to internal overpressure upstream of the silencer.</b></p> <p>Inadmissibly high pressure upstream of the silencer can cause the vacuum pump to burst or damage seals.</p> <p>Internal overpressure can occur when the gas flow rate is high or there are deposits in the silencer due to the pumping of gases containing dust or solvent vapors.</p> <ul style="list-style-type: none"> <li>⇒ Do not pump any substances that could form deposits inside the silencer.</li> <li>⇒ If the gas flow rate is permanently high or there is a risk of deposits, do not use a silencer at the outlet. Instead, connect an outlet line to small flange KF DN 25.</li> </ul>

⇒ Connect the silencer with small flange KF DN 25 to the outlet flange, ensuring the connection is gas-tight.


Vacuum pump with  
mounted silencer



### 4.3.3 Electrical connection

#### Connect the vacuum pump electrically

→ Example  
Electrical connection  
for vacuum pump

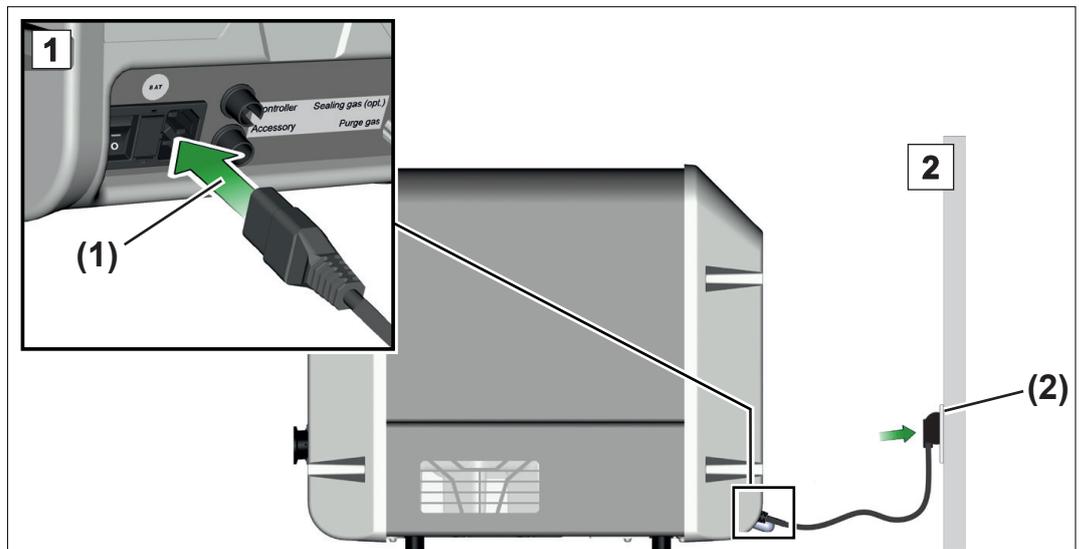

1. Plug connector (1) of the power cord into the power connection of the vacuum pump.
2. Plug power plug (2) into the power outlet.
  - Vacuum pump electrically connected.

- ⇒ Lay the power cord such that it cannot be damaged by sharp edges, chemicals, or hot surfaces.
- ⇒ The power plug serves as a disconnecting device from the electrical supply voltage. The product must be installed in such a way that the power plug is easily reached and accessible at all times to disconnect the product from the power supply.

#### Power connection

The vacuum pump is delivered ready for use with the appropriate power plug.


- ⇒ Use the power plug which fits your power connection.
- ⇒ Do not use multiple sockets connected in series as the power connection.

## 5 Commissioning (operation)

### 5.1 Switch on

#### Switch on the vacuum pump

Switch on the vacuum pump

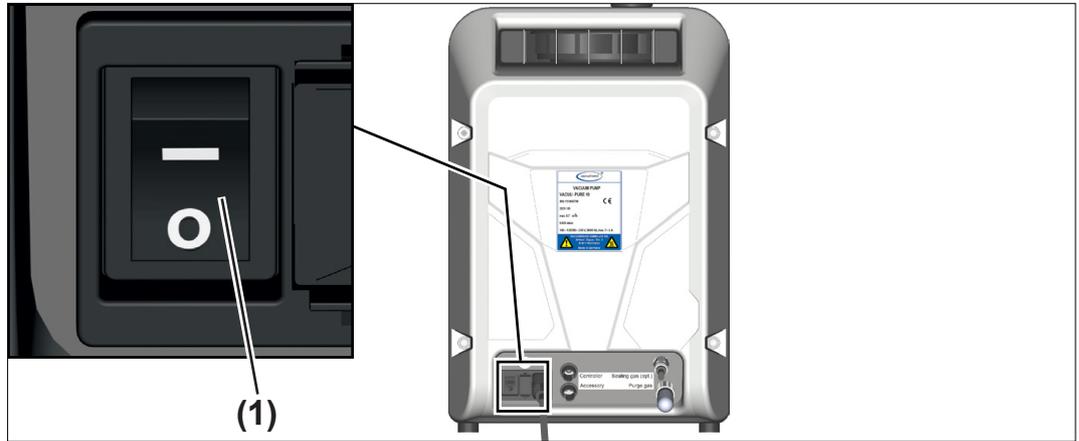

⇒ Switch rocker switch (1) on – switch position I.


- ☑ The vacuum pump carries out a function test; all LEDs light up for 2 seconds. The stop button's blue LED will then light up.

The vacuum pump is ready for operation immediately after switching on.

### 5.2 Operation

#### Control panel

Control panel

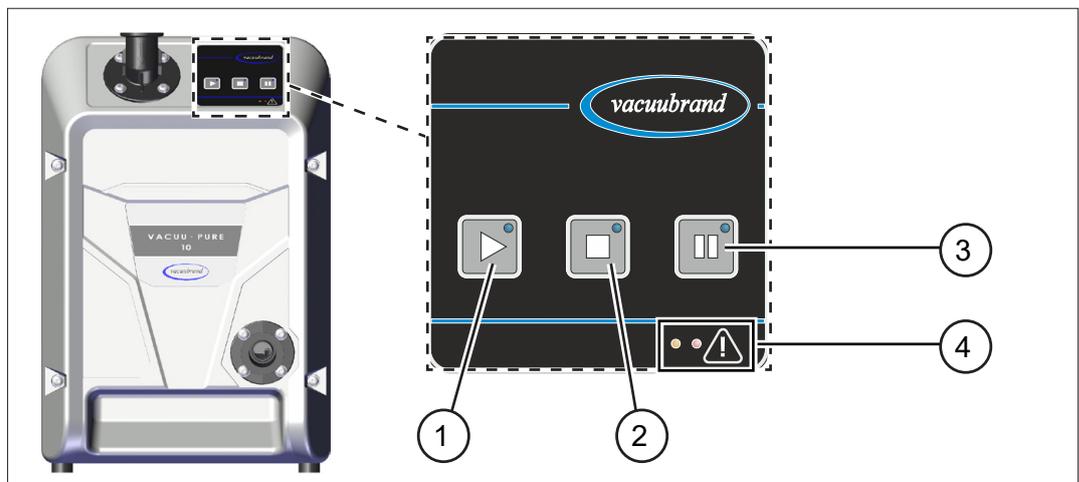

- 1 Start vacuum pump
- 2 Stop vacuum pump
- 3 Regeneration mode (vacuum pump drying)
- 4 LEDs warning (left / yellow) / error (right / red)


## Operating elements

Operating elements

Button	Operating elements
	Start vacuum pump
	Stop vacuum pump
	Vacuum pump regeneration mode (vacuum pump starts/ continues running at reduced speed)

## Display elements

Display elements

Button LED	Description
	 Vacuum pump running
	 Vacuum pump stopped
	 Vacuum pump regeneration mode activated

Button LED	Description
All	 Function not active
	 Short flashing  = visual feedback when key is pressed
	Continuous light = indication for active mode


LED warning / error	Description
 Gray	No warning or error active
 Yellow	Flashing rate  = warning
	Continuous light when software version is displayed
 Red	Flashing rate  = error
	Continuous light when hardware version is displayed

### 5.2.1 Operation

#### Start the vacuum pump

**IMPORTANT!**

⇒ Make sure that the outlet is clear and non-pressurized.

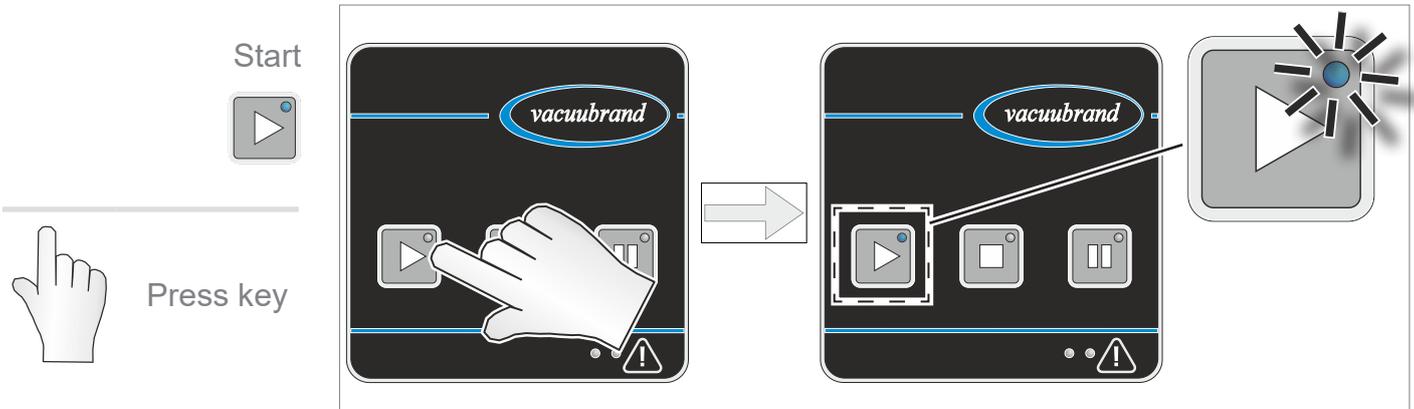

- ☑ The vacuum pump starts. A clicking switch noise can be heard briefly.

#### Warm-up (warm-up time)


Warm-up time

The operating principle of the vacuum pump is based on gap seals.

⇒ The warm-up time enables the vacuum pump to reach full operating capacity. When pumping down a 100 l boiler, the vacuum pump typically reaches the specified ultimate vacuum after 20 minutes.

<b>VACUU·PURE 10</b>	Warm-up time (vacuum pump started)	▶ 20 minutes
----------------------	------------------------------------	--------------

#### Stop the vacuum pump

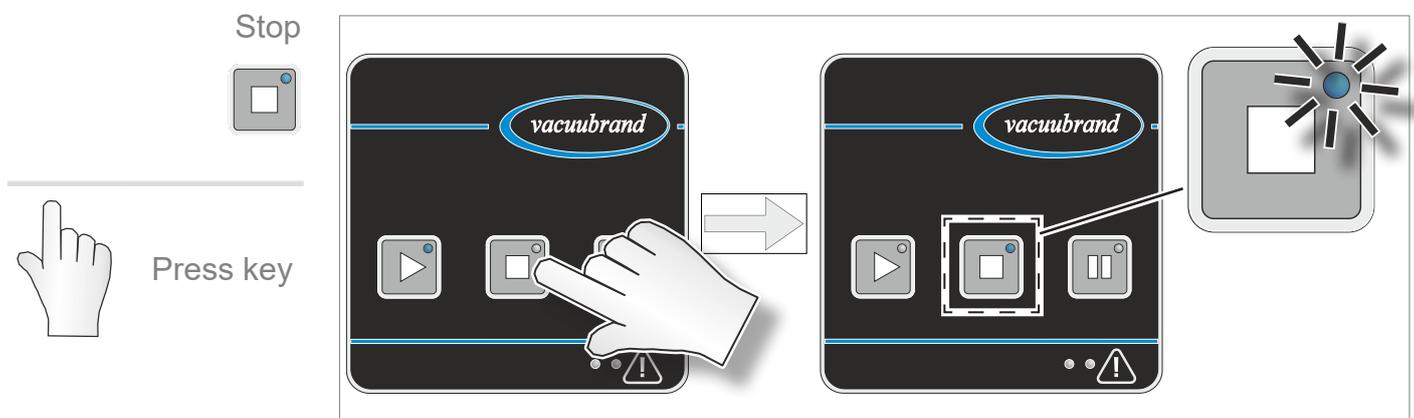

- ☑ The vacuum pump stops. A clicking switch noise may be heard briefly.

## IMPORTANT!

- ⇒ The vacuum pump does not create a vacuum-tight seal when it switches off.
- ⇒ If necessary, install an in-line solenoid valve or shut-off valve in the inlet line to isolate your application from the vacuum pump with a vacuum-tight seal.

### 5.2.2 Regeneration mode

Drying  
(regeneration) with  
ambient air

Regeneration mode is used to quickly dry the pump interior after the application is finished or before it is taken out of service. Here, ambient air is fed into the interior of the pump and the interior is dried by the air supply.


- The pump does not need to be separated from the application for regeneration.
- The pump runs at a reduced speed during regeneration.
- The air for regeneration mode is drawn in via a filter on the rear of the vacuum pump. The ambient air is aspirated here.

⇒ Check the filter regularly for dirt and blockages.

⇒ Replace dirty or clogged filters

→ see chapter: 7.3 Air inlet filter on page 68.

### Start regeneration mode

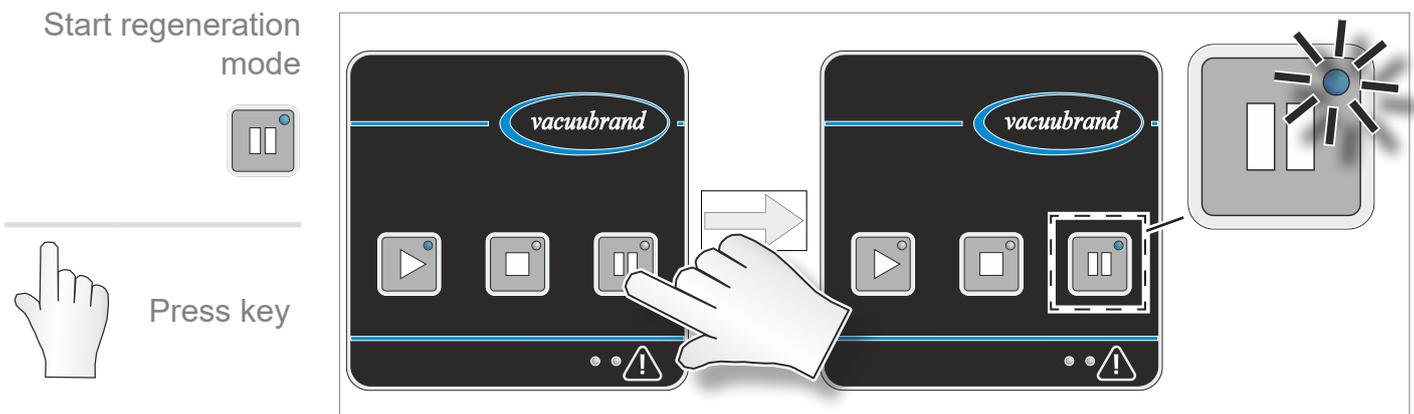

- The vacuum pump runs at a reduced speed and aspirates ambient air.
- The inside of the pump is dried.
- Regeneration mode ends automatically after a period of one hour.

## Dry the vacuum pump before changing media

Dry vacuum pump

The vacuum pump can be dried with the aspirated ambient air without having to be separated from the application / equipment.

⇒ Use regeneration mode before changing the pumped medium or the connected process, if pumped media can react with each other in the vacuum pump or form deposits.

## Dry the vacuum pump after process end

The vacuum pump can be dried with the aspirated ambient air.

⇒ Use the vacuum pump's regeneration mode after the end of the process before stopping or switching off the vacuum pump.

⇒ Allow the vacuum pump to continue running in regeneration mode for about 30 minutes after the end of the process. This reduces condensate and media residue in the vacuum pump and thus also the risk of impairment to the vacuum pump by the previously pumped media.

### 5.2.3 Autostart

Autostart  
automatic restart of  
the vacuum pump

The vacuum pump has an Autostart function. When the power supply is switched off and then back on, the last active operating state of the vacuum pump is automatically reactivated:

#### Operating status of the vacuum pump:

before discontinuation of mains voltage	after restoration of mains voltage
Vacuum pump started	Vacuum pump starts automatically
Vacuum pump stopped	Vacuum pump stopped
Regeneration mode active	Regeneration mode automatically active

⇒ Stop the vacuum pump with the stop button before switching off the power switch or pulling the power plug.

☑ This is how you will avoid an unintentional or unexpected start of the vacuum pump the next time it is switched on.

### 5.3 Advanced operation



In addition to the simple operation of the vacuum pump – start, stop, regeneration – you can carry out other functions by pressing and holding individual keys or by combining them.

#### 5.3.1 Display of software / hardware version

Display of software / hardware version



Keep key pressed

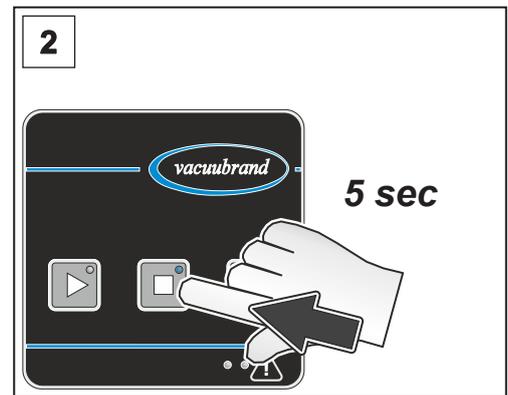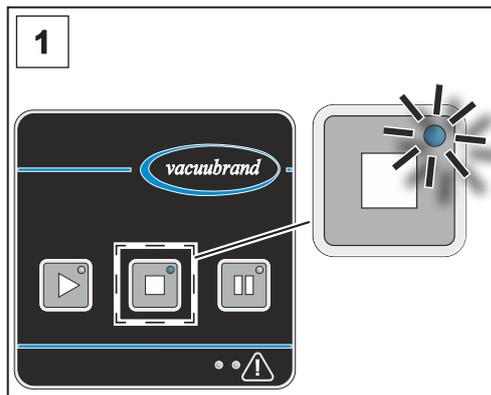

1. The vacuum pump is switched on and stopped.

2. Press and hold the stop button for 5 seconds.

⇒ The warning and error LEDs indicate whether the software or hardware version is currently being displayed:



▪ Yellow LED (left) for warning lights up: Software version displayed






▪ Red LED (right) for errors lights up: Hardware version displayed

⇒ The software version and the hardware version are indicated alternately by successive flashing of the LEDs on the operating buttons.

## Example

Display of software version V1.23 (LED on left, yellow) and hardware version V1.05 (LED on right, red):

LEDs	Description / flashing rate
	Software version display (1 second)
	 1x $\square$ = V 1.XX
	 2x $\square$ = V X.2X
	 3x $\square$ = V X.X3
	3 seconds pause, LED changes from yellow to red
	Hardware version display (1 second)
	 1x $\square$ = V 1.XX
	 Not flashing = V X.0X
	 5x $\square$ = V X.X5
	3 seconds pause – then the display starts again from the beginning

⇒ Exit the display by briefly pressing the stop button or automatically after 5 minutes.

## 5.3.2 Restore factory settings


Restore factory settings

When restoring the factory settings, any changes made by the customer – mainly with accessories optionally connected via VACUU·BUS – will be reset to factory settings.


⇒ The software version of the vacuum pump is retained and is not reset.




Keep key pressed

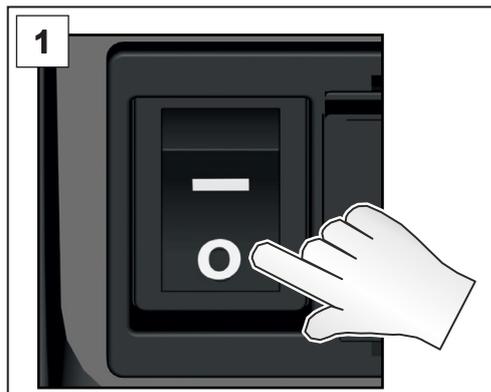


1. Turn off the power switch. Wait 10 seconds until the vacuum pump is completely off.

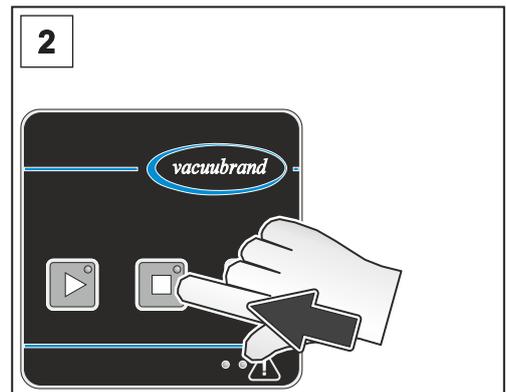


2. The vacuum pump is switched off. Press and hold the stop button.

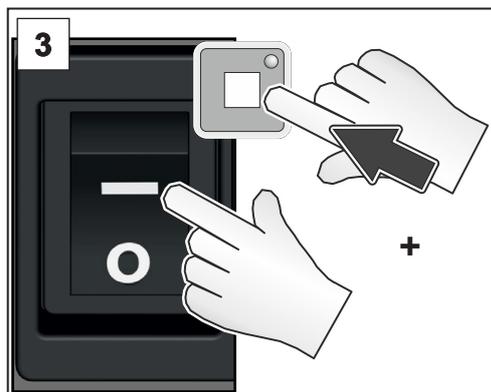

3. Turn on the power switch while continuing to hold down the stop button.

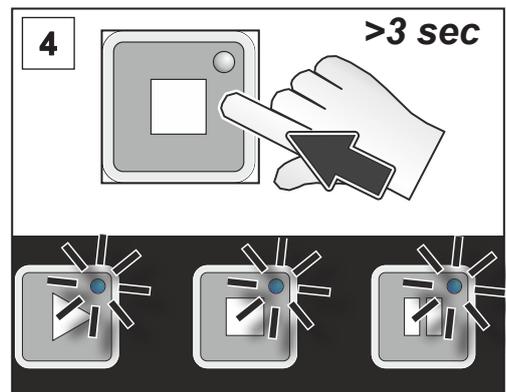

4. Continue to hold down the stop button for another 3 seconds until all button LEDs flash, then release the stop button.

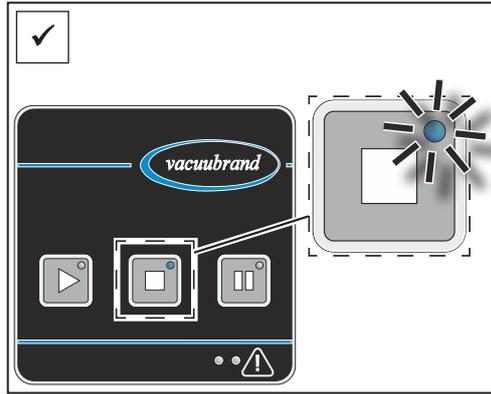

- The stop button lights up continuously. The vacuum pump's factory settings are restored.


### 5.3.3 Remote operation via Modbus RTU

Modbus RTU:  
Remote operation  
and parameter  
setting

The upper VACUU·BUS port on the back of the vacuum pump is intended for remote operation of the vacuum pump, via Modbus RTU protocol. Via the Modbus RTU protocol, parameters of the vacuum pump (Autostart) and of VACUU·BUS accessories can also be set → *see separate manual for description of the Modbus RTU interface.*

## 5.4 Connect / remove VACUU-BUS accessories

### Connect VACUU-BUS accessories



Connect  
VACUU-BUS  
accessories

1. Stop the vacuum pump and switch off the vacuum pump at the power switch.
2. Insert the VACUU-BUS plug of the accessory into the lower socket on the back of the vacuum pump.
3. Switch on the vacuum pump at the power switch. The connected accessories are automatically detected.

VACUU-BUS accessories connected.

### Remove VACUU-BUS accessories

Remove  
VACUU-BUS  
accessories

1. Stop the vacuum pump and switch off the vacuum pump at the power switch.
2. Unplug the VACUU-BUS accessories on the back of the vacuum pump.
3. Carry out a bus scan of the vacuum pump to deregister the accessories from the vacuum pump bus system → see *chapter: 5.4.1 VACUU-BUS detection on page 52*.

VACUU-BUS accessories removed.

### General notes on VACUU-BUS components

VACUU-BUS  
accessories –  
General information

- Use Y adapters and extension cables to connect and use several VACUU-BUS components in parallel.
- A maximum of six VACUU-BUS components can be connected and used in parallel.
- A maximum of four components of the same type can be connected.
- Each connected VACUU-BUS component must have a different VACUU-BUS address. The connection of two components with identical VACUU-BUS addresses leads to errors in the bus system. (Reconfiguration of the VACUU-BUS address of a component: see manual of a **VACUUBRAND** controller, e.g., VACUU-SELECT).
- Note the maximum permissible load of 11 W at the VACUU-BUS port.

- Maximum permissible cable length in the VACUU·BUS system: 30 m.
- An interruption in communication with accessories or the removal of accessories causes the vacuum pump to stop immediately and an error message to be displayed (flashing rate: 6x) → see *chapter: 6.3.2 Error – Cause – Remedy on page 59*.


## 5.4.1 VACUU·BUS detection

### Perform bus scan (VACUU·BUS)


Perform bus scan




Keep key pressed

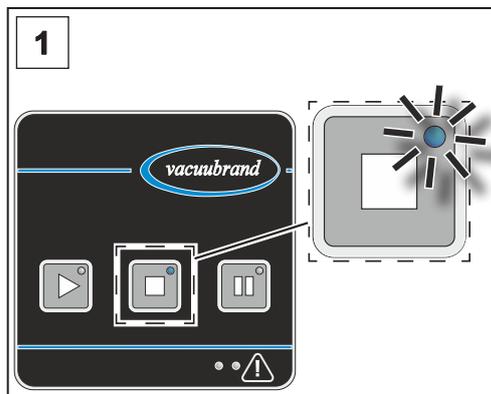


1. The vacuum pump is switched on and stopped.

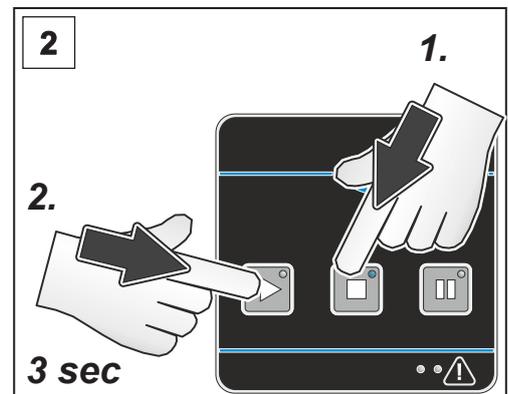

2. First hold down the stop button and then also hold down the start button for 3 seconds.

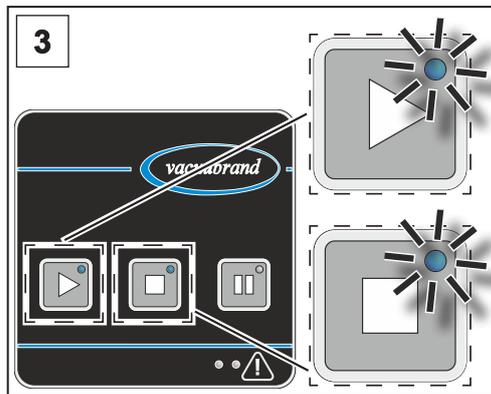

3. The LEDs for the stop and start buttons flash for 5 seconds.

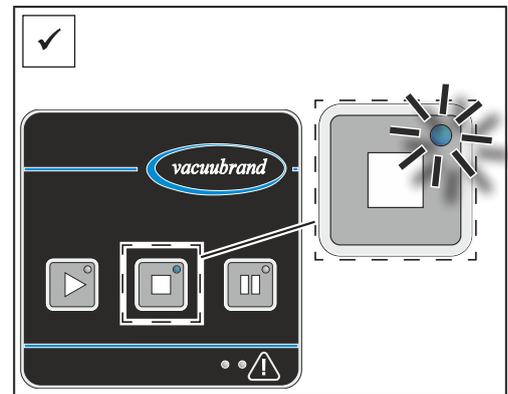

☑ The stop button lights up. The bus scan is completed. The connected accessories are detected.

## 5.4.2 Operation with VACUU·BUS accessories

### Operation with in-line solenoid valve

Operation with  
in-line solenoid  
valve

- The in-line solenoid valve automatically opens 10 seconds after the start button is pressed. The value of the waiting time can be set via the Modbus RTU protocol: 0 – 3600 seconds.
- The in-line solenoid valve closes immediately after pressing the stop button or the regeneration button.

### Operation of vacuum gauge VACUU·VIEW (extended)

Operation with  
VACUU·VIEW  
(extended)

- Use a VACUU·VIEW (extended) to display the current pressure in the application or at the inlet or outlet of the vacuum pump.
- The pressure display starts automatically when the vacuum pump is switched on.

## 5.5 Shutdown (switch off)

Shutdown **Take the vacuum pump out of operation**

1. Stop the process.


### IMPORTANT!

⇒ Avoid deposits and dry the vacuum pump in regeneration mode.

- ✓ By letting the vacuum pump run on in regeneration mode, you reduce condensate and media residue in the vacuum pump.
- ✓ You reduce the risk of a possible impairment of the vacuum pump by the previously pumped media by letting the vacuum pump run on.




Press key

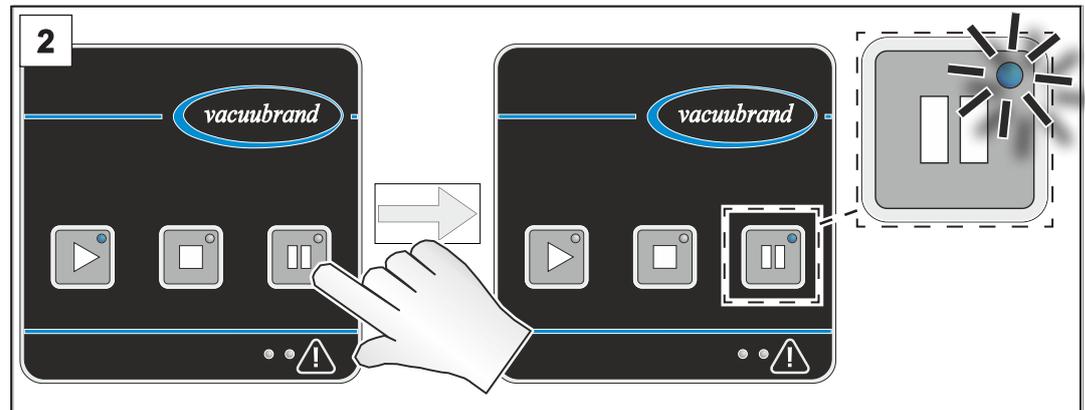


2. Allow the vacuum pump to run on for about 30 minutes in regeneration mode.



Press key

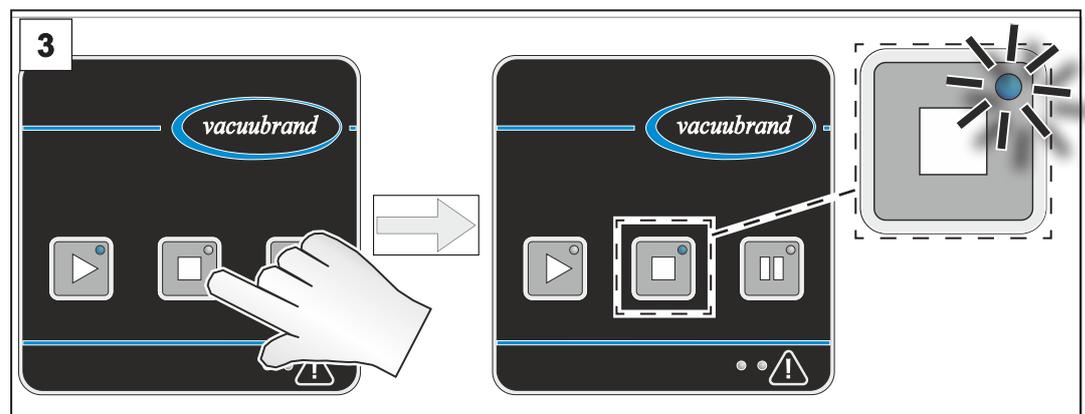

3. Stop the vacuum pump.

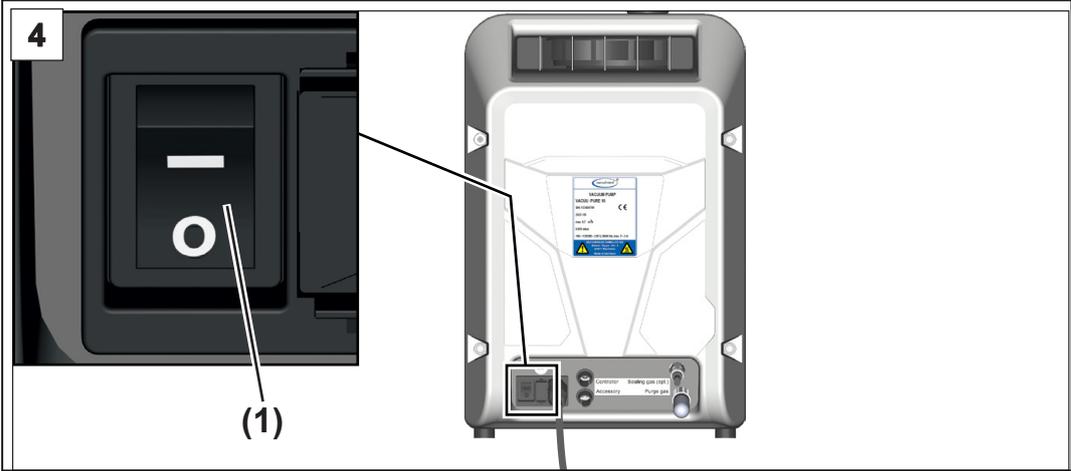

4. Switch off rocker switch (1) – switch position 0.
  - Vacuum pump switched off.
5. Disconnect the vacuum pump from the apparatus.
6. Check the vacuum pump for possible damage and contamination.

### 5.6 Storage

#### Store the vacuum pump

Store the vacuum pump

1. Carry out the steps for decommissioning → see *chapter: 5.5 Shutdown (switch off) on page 54.*
2. Clean the vacuum pump in the event of external contamination.
3. Close the vacuum pump's inlet and outlet, e.g., with the transport locks.
4. Package the vacuum pump such that it is protected from dust; enclose desiccants if necessary.
5. Store the vacuum pump in a cool, dry location.


**IMPORTANT!**

If damaged parts are stored for operational reasons, these should be clearly identified as **not ready for use.**

## 6 Error messages

General error messages


Errors or warnings are indicated by the colored LEDs on the warning triangle. Several error messages may be pending at the same time. Errors and warnings can be identified via the flashing rate.

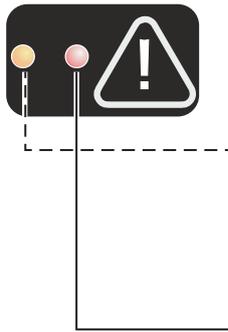

LED	Description
 Gray	No warning or error active
 Yellow	<b>Warning</b> Warning messages reset themselves as soon as the values are back within the normal range. The vacuum pump continues to run if a warning message is received.
 Red	<b>Error</b> The vacuum pump stops as soon as there is an error. If there is an error, all warnings are ignored. First correct the error before resetting.

### 6.1 Warning display

Possible flashing rates in the event of a warning

Flashing	Description
1x 	Temperature in critical range
2x 	Not assigned
3x 	Motor current consumption in critical range
4x 	Fan speed deviation
5x 	Supply voltage for control board in critical range
6x 	Messages: VACUU·BUS accessories (e.g., overpressure of a vacuum sensor)
7x 	Other warnings

## 6.2 Error indication


Possible flashing rates in the event of an error

Flashing	Description
1x 	Temperature in the inadmissible range
2x 	Not assigned
3x 	Motor current consumption in faulty range or other motor error
4x 	Fan defective
5x 	Overvoltage or undervoltage in the intermediate circuit of the frequency converter
6x 	Error / communication interruption VACUU·BUS accessories
7x 	Other errors (software versions of control board/ frequency converter incompatible with each other; other frequency converter errors)

- ⇒ If warnings and errors occur simultaneously, only the errors (red LED) are displayed.
- ⇒ Several errors are indicated one after the other by combined flashing cycles.
- ⇒ An error message is displayed until it is acknowledged. Acknowledge an error message by switching the power switch off and on after you have eliminated the error.

### Example

→ Example  
Pending error

Error	LED flashing rate 
Temperature error (1x) and other errors (7x) occur at the same time	

Which and how many errors are present can be identified from the flashing cycles.

## 6.3 Troubleshooting

### 6.3.1 Technical support

⇒ To identify errors and potential remedies, please refer to the troubleshooting table

***Error – Cause – Remedy.***

Technical  
support

For technical assistance or errors for which you require additional support, please contact your local distributor or our [Service Department](#)<sup>1</sup>.



Only operate the product if it is in perfect working condition.

- ⇒ Perform the recommended service activities → see ***chapter: 7.1 Information on maintenance work on page 66***, and ensure that the product is in good working order.
- ⇒ Send defective products to our Service Department or your local distributor for repair!

<sup>1</sup> -> Phone: +49 9342 808-5660, fax: +49 9342 808-5555, [service@vacuubrand.com](mailto:service@vacuubrand.com)

## 6.3.2 Error – Cause – Remedy

Error – Cause –  
Remedy

Error	▶ Possible cause	✓ Remedy	Personnel
Warning flashing rate 1x	▶ Ambient temperature increased.	<ul style="list-style-type: none"> <li>✓ Observe the vacuum pump's limitation of use.</li> <li>✓ Ensure a supply of cooling air.</li> </ul>	Specialist
	▶ Minimum clearances not observed when installed in lab furniture.	<ul style="list-style-type: none"> <li>✓ Maintain minimum clearances to adjacent objects or surfaces.</li> </ul>	
	▶ Cooling air supply blocked; fan grilles dirty.	<ul style="list-style-type: none"> <li>✓ Ensure a supply of cooling air.</li> <li>✓ Clean the fan grilles.</li> </ul>	
	▶ Cooling air outlet blocked.	<ul style="list-style-type: none"> <li>✓ Check and clear the cooling air outlet. Ensure cooling air outlet is kept clear.</li> </ul>	
	▶ Power supply too low, undervoltage.	<ul style="list-style-type: none"> <li>✓ Check mains voltage.</li> </ul>	
	▶ Pumping down hot process gases.	<ul style="list-style-type: none"> <li>✓ Observe admissible gas intake temperatures.</li> </ul>	
Warning flashing rate 3x	▶ Motor current consumption in critical range, deposits in pump unit due to pumped media.	<ul style="list-style-type: none"> <li>✓ Clean the pump unit by operating it with an open inlet or in regeneration mode.</li> </ul>	Operator
Warning flashing rate 4x	▶ Fan speed deviation.	<ul style="list-style-type: none"> <li>✓ Remove possible blockage in the cooling air outlet.</li> </ul>	Operator
Warning flashing rate 5x	▶ Supply voltage for control board in critical range.	<ul style="list-style-type: none"> <li>✓ Remove any connected VACUU·BUS accessories if too many or replace if faulty.</li> </ul>	Specialist
Warning flashing rate 6x	▶ Message: VACUU·BUS accessories (vacuum sensor overpressure).	<ul style="list-style-type: none"> <li>✓ Check pressure in system and reduce if necessary.</li> <li>✓ Check vacuum sensor, calibrate if necessary. Replace defective sensor.</li> </ul>	Operator

Error – Cause –  
Remedy

<b>Error</b>	<b>▶ Possible cause</b>	<b>✓ Remedy</b>	<b>Personnel</b>
Warning flashing rate 7x	▶ Other warnings.	✓ Send in vacuum pump.	Resp. specialist
Error flashing rate 1x	▶ Ambient temperature increased.	✓ Observe the vacuum pump's limitation of use. ✓ Ensure a supply of cooling air.	Resp. specialist
	▶ Minimum clearances not observed when installed in lab furniture.	✓ Maintain minimum clearances to adjacent objects or surfaces.	
	▶ Cooling air supply blocked; fan grilles dirty.	✓ Ensure a supply of cooling air. ✓ Clean the fan grilles.	
	▶ Cooling air outlet blocked.	✓ Check and clear the cooling air outlet. Ensure cooling air outlet is kept clear.	
	▶ Power supply too low, undervoltage.	✓ Check mains voltage.	
	▶ Pumping down process gases that are too hot.	✓ Observe admissible gas intake temperatures.	
Error flashing rate 3x	▶ Motor current consumption in faulty range, deposits in the pump unit due to pumped media.	✓ Clean the pump unit by operating it with an open inlet or in regeneration mode.	Operator
	▶ Motor current consumption in faulty range or other motor error.	✓ In case of unusual operating noises: Send in vacuum pump.	Resp. specialist
Error flashing rate 4x	▶ Fan jammed.	✓ Remove mechanical blockage from fan. ✓ Remove blockage in cooling air outlet.	Resp. specialist
	▶ Fan defective.	✓ Send in vacuum pump.	
Error flashing rate 5x	▶ Overvoltage or undervoltage in intermediate circuit (frequency converter).	✓ Check mains voltage. ✓ Send in vacuum pump.	Resp. specialist

Error – Cause – Remedy

Error	▶ Possible cause	✓ Remedy	Personnel
Error flashing rate 6x	▶ VACUU·BUS accessories removed / unplugged.	<ul style="list-style-type: none"> <li>✓ Plug in VACUU·BUS accessories again and switch vacuum pump off/on.</li> <li>✓ Operation without VACUU·BUS accessories: Perform bus scan.</li> </ul>	Operator
	▶ Error or communication interruption in VACUU·BUS accessories.	<ul style="list-style-type: none"> <li>✓ Check VACUU·BUS plug-in connection to accessories.</li> <li>✓ Replace defective components.</li> </ul>	
Error flashing rate 7x	▶ Other errors (e.g., incompatible software version, other frequency converter errors).	<ul style="list-style-type: none"> <li>✓ Perform or repeat the software update. Information about software updates: <a href="#">VACUUBRAND &gt; Support &gt; Software Updates</a></li> <li>✓ Send in vacuum pump.</li> </ul>	Resp. specialist
Optional accessories: Vacuum sensor does not display a measured value.	▶ No voltage applied.	✓ Apply mains voltage, switch on vacuum pump.	Operator
	▶ VACUU·BUS plug-in connection or cables defective or not connected.	✓ Check VACUU·BUS plug-in connection and wiring.	
	▶ External plug-in power supply of vacuum sensor not plugged in.	✓ Plug-in power supply for vacuum sensor.	
	▶ Sensor defective.	✓ Replace defective components.	Specialist

Error – Cause –  
Remedy

<b>Error</b>	<b>▶ Possible cause</b>	<b>✓ Remedy</b>	<b>Personnel</b>
Vacuum pump does not start.	▶ Vacuum pump switched off.	✓ Switch on vacuum pump at toggle switch.	Operator
	▶ Power plug not correctly plugged in or pulled out.	✓ Check power connection and cable.	
	▶ Overpressure in the outlet line.	✓ Open the outlet line.	
	▶ External silencer (optional) clogged or jammed.	✓ Clean or replace external silencer. ✓ Remove silencer and connect outlet line instead.	Resp. specialist
	▶ Motor overloaded.	✓ Allow the motor to cool down.	
	▶ Excessive temperature error flashing rate 1x.	✓ See error, flashing rate 1x.	
	▶ Vacuum pump mechanically blocked.	✓ Send in vacuum pump.	
Ultimate vacuum not reached.	▶ Leak in inlet line or in apparatus.	✓ Check inlet line and equipment for leaks.	Operator
	▶ Vacuum pump not at operating temperature.	✓ Allow vacuum pump to warm up for 20 minutes with inlet closed.	
	▶ Leak inside vacuum pump.	✓ Send in vacuum pump.	Resp. specialist

Error – Cause – Remedy

<b>Error</b>	<b>▶ Possible cause</b>	<b>✓ Remedy</b>	<b>Personnel</b>
No suction power or minimal suction power.	▶ Leak in inlet line or in apparatus.	✓ Check inlet line and equipment for leaks.	Operator
	▶ Inlet line too long or cross-section too small.	✓ Use shorter inlet line with larger cross-section.	
	▶ Condensate inside the vacuum pump.	✓ Let vacuum pump run for a few minutes with suction nozzle open or in regeneration mode.	
	▶ Deposits inside the vacuum pump.	✓ Clean the pump unit by operating it with an open inlet or in regeneration mode.	
	▶ High level of vapor generated in the process.	✓ Check process parameter.	Specialist
	▶ Pump speed reduced due to excessive temperature.	✓ See warning, flashing rate 1x.	Resp. specialist
Key LEDs do not light up	▶ Vacuum pump switched off.	✓ Switch on vacuum pump at toggle switch.	Operator
	▶ Power plug not correctly plugged in or pulled out.	✓ Check power connection and cable.	
	▶ Vacuum pump defective.	✓ Send in vacuum pump.	Resp. specialist

Error – Cause –  
Remedy

<b>Error</b>	<b>▶ Possible cause</b>	<b>✓ Remedy</b>	<b>Personnel</b>
Loud operating noises	▶ No outlet line connected.	✓ Check outlet line and connect it correctly. ✓ Connect optional external silencer at the outlet; <i><b>see chapter: 8.2 Ordering information on page 76.</b></i>	Operator
	▶ Internal non-return valve switches.	✓ Normal when starting and stopping vacuum pump.	
	▶ Internal non-return valve opens and closes several times.	✓ Normal behavior under unfavorable pressure conditions at the inlet.	
	▶ Mechanical defect of vacuum pump, e.g., defective ball bearing.	✓ Send in vacuum pump.	Resp. specialist
	▶ Internal silencer clogged.	✓ Send in vacuum pump.	

## 7 Cleaning and maintenance

	<p><b>WARNING</b></p>
	<p><b>Danger due to electrical voltage.</b></p> <ul style="list-style-type: none"> <li>⇒ Switch the product off before cleaning or maintenance work.</li> <li>⇒ Unplug the power plug from the socket.</li> </ul>
	<p><b>Risk from contaminated parts.</b></p> <p>Pumping hazardous media can result in hazardous substances adhering to internal parts of the pump.</p> <ul style="list-style-type: none"> <li>⇒ Wear your personal protective equipment, e.g., protective gloves, eye protection and, if necessary, respiratory protection.</li> <li>⇒ Take safety precautions according to the instructions you have received on handling hazardous substances.</li> </ul>

<p><b>NOTE</b></p>	
<p><b>Damage possible if work is performed incorrectly.</b></p> <ul style="list-style-type: none"> <li>⇒ Have maintenance work performed by a trained specialist or at least by a trained person.</li> <li>⇒ Recommendation: Before carrying out maintenance work for the first time, please read through all the handling instructions to get an overview of the required service work.</li> </ul>	

## 7.1 Information on maintenance work

### Recommended maintenance activities

Maintenance intervals

Maintenance intervals	As required
Clean surfaces	X
Clean / vacuum fan grilles	X
Clean the vacuum pump	X
Replace filter at air inlet for regeneration mode	X

### Recommended aids

→ Example  
Recommended aids



No.	Item
1	Safety goggles
2	Protective gloves
3	Vacuum cleaner

### IMPORTANT!

⇒ Always wear your personal protective equipment when performing activities which may bring you into contact with hazardous substances.

## 7.2 Cleaning

This chapter does not contain descriptions for decontamination of the product. This chapter describes simple measures for cleaning and care.

⇒ Switch off vacuum pump before cleaning.

### 7.2.1 Clean the vacuum pump

#### Clean surfaces




⇒ Clean dirty surfaces with a clean, slightly damp cloth. We recommend using water or mild soapy water to moisten the cloth.

#### Clean the fan grilles

Clean the fan grilles

The fan grilles (2 pieces) are located on the right and left side of the pump.

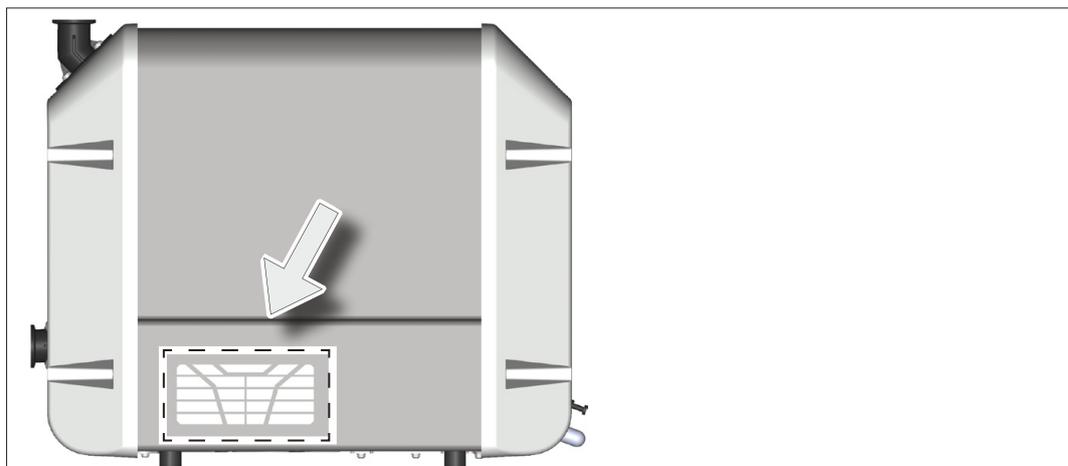


⇒ Clean dirty fan grilles, for example with a vacuum cleaner.

### 7.3 Air inlet filter

Replacement of air inlet filter (regeneration mode)


Position of the filter (air inlet for regeneration mode) on the vacuum pump:

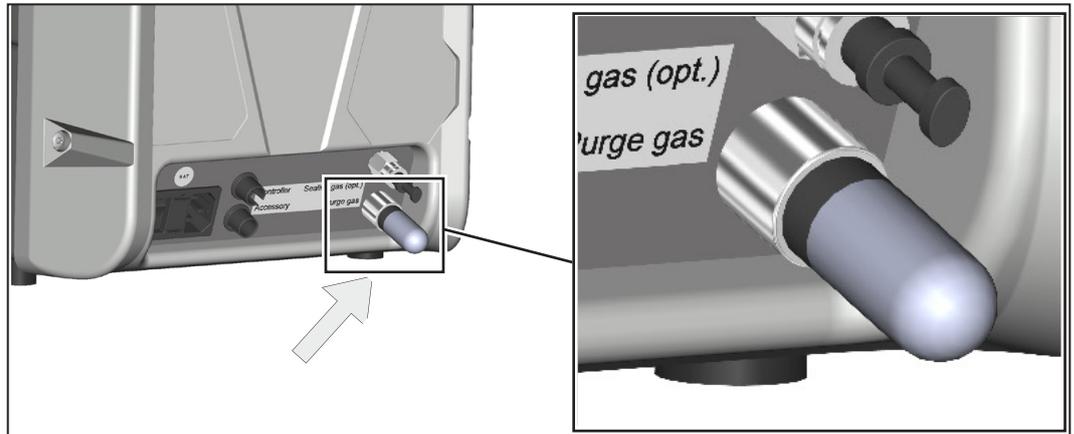


⇒ Replace a dirty or clogged air filter at the air inlet for regeneration mode.

The filter is available as a spare part → see *chapter: 8.2 Ordering information on page 76*.

#### Replace filter at air inlet (regeneration mode)

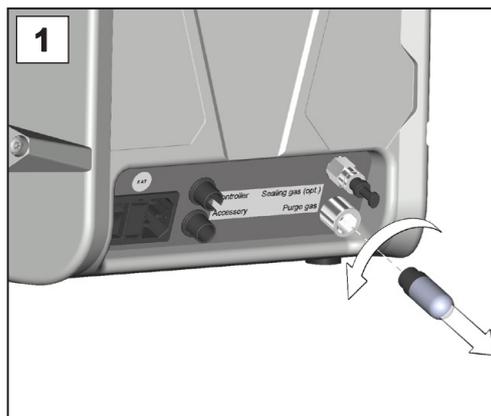

1. Unscrew the dirty filter at the purge gas inlet.

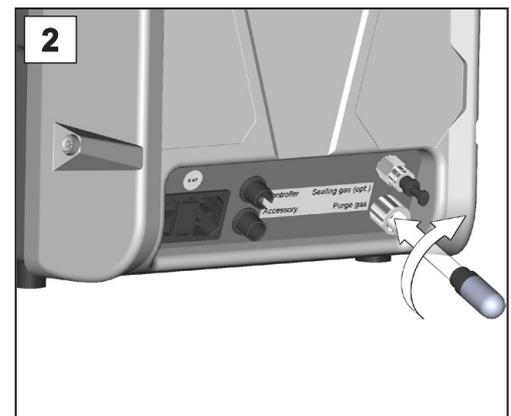


2. Screw in the new filter at the purge gas inlet.

**7.4 Replace the device fuse**

Replace the device fuse

You will find 2 device fuses at the power connection on the back of the vacuum pump, type: 8 AT – 5x20

**Replace the device fuse**

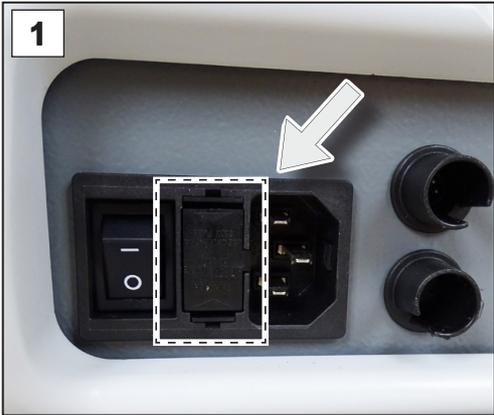


1. Unplug the power plug. The mains fuses are located in a fuse holder next to the on/off switch.



2. Keep the snap hooks pressed down. Carefully pull out the fuse holder.



3. Replace the fuses.

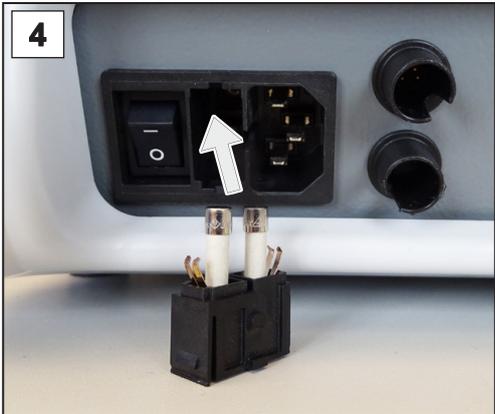

4. Slide the fuse holder onto the fuse base until it clicks into place.

## 8 Appendix

### 8.1 Technical information

#### 8.1.1 Technical data

##### Vacuum pump

Vacuum pump  
technical data

<b>Ambient conditions</b>		(US)
Ambient temperature, max.	10 – 40 °C	50 – 104 °F
Storage/transport temperature	-10 – 60 °C	14 – 140 °F
Max. altitude	2000 m above sea level	6562 ft above sea level
Relative humidity	30 – 85 %, non-condensing	
Pollution degree	2	
Impact energy	5 J	
Protection class (DIN 60529)	IP 20	
Protection class (UL 50E)	NEMA type 1	

<b>Operating conditions</b>		(US)
Maximum admissible media temperature (gas), non-explosive atmosphere:		
Short term	80 °C	176 °F
Continuous operation	40 °C	104 °F
Max. surface temperature in the area in contact with the medium	160 °C	320 °F

<b>Connections</b>	
Vacuum connection IN (inlet)	Small flange KF DN 25
Outlet connection OUT	Small flange KF DN 25
Cold device plug	+ power connection CEE, CH, CN, UK, IN, US
Connection accessories (optional)	VACUU·BUS
Controller connection (optional)	VACUU·BUS / Modbus RTU

## Technical data

<b>Electrical data</b>	
Nominal voltage	100 – 230 V $\pm$ 10 %
Mains frequency	50 / 60 Hz
Overvoltage category	II
Power, max.	700 W
Interface	VACUU·BUS / Modbus RTU
Power cord	2 m
Max. permissible load on VACUU·BUS connections	11 W
Device fuse 2x	8 AT 5x20

<b>Vacuum data</b>		(US)
Max. pumping speed	10 m <sup>3</sup> /h	5.9 cfm
Ultimate vacuum*, abs.	5*10 <sup>-3</sup> mbar	3.8*10 <sup>-3</sup> Torr
Max. inlet pressure, abs.	Atmospheric pressure (ATM)	
Max. outlet pressure, abs.	15 mbar above atmospheric pressure	11 Torr above atmospheric pressure

\* Specification at 1013 mbar. Due to their functional principle, the ultimate vacuum of screw pumps of this design shows a dependency on the ambient pressure.

<b>Mechanical data</b>		(US)
Dimensions (L x W x H)	507 mm x 269 mm x 413 mm	20 in x 10.6 in x 16.3 in
Weight*	21.1 kg	46.5 lb

\* without cable

<b>Other information</b>	
Emission sound pressure level* (uncertainty K <sub>pA</sub> : 3 dB(A))	55 dB(A)

\* Measurement according to DIN EN ISO 2151:2009 and EN ISO 3744:1995 at ultimate vacuum with outlet line at outlet connection


## Frequency converter

Frequency converter  
technical data

<b>Frequency converter</b>		
Type	FC 700S 10	
<b>Ambient conditions</b> (US)		
Ambient temperature, max. (end use)	10 – 40 °C	50 – 104 °F
Storage/transport temperature	-10 – 60 °C	14 – 140 °F
Installation height, maximum (end use)	2000 m above sea level	6562 ft above sea level
Relative humidity	30 – 85 %, non-condensing	
Pollution degree	2	
Protection class (DIN 60529) (end use)	IP 00	
EMC (DIN EN 61326) (end use)	CE Declaration	
Cooling (end use)	Actively cooled	
<b>Electrical data</b>		
Nominal voltage	100 – 230 V ±10 %	
Mains frequency	50 / 60 Hz	
Power, max.	700 W	
Output voltage	max. 400 VDC phase–phase	
<b>Mechanical data</b> (US)		
Housing	Open aluminum housing (drawer unit in end use)	
Dimensions (L x W x H)	220 mm x 253 mm x 119 mm	8.7 in x 10 in x 4.7 in
Weight including housing	1.96 kg	4.3 lb
<b>Interfaces</b>		
I/O interfaces	RS-485	
Internal power supply unit	24 VDC, 25 W (SELV)	
<b>Function</b>		
Software	Programming / parameterization	
Protective function	Overvoltage / undervoltage in the intermediate circuit; overcurrent; excessive temperature	

**Overview of frequency converter board**

Inputs and outputs on the frequency converter board

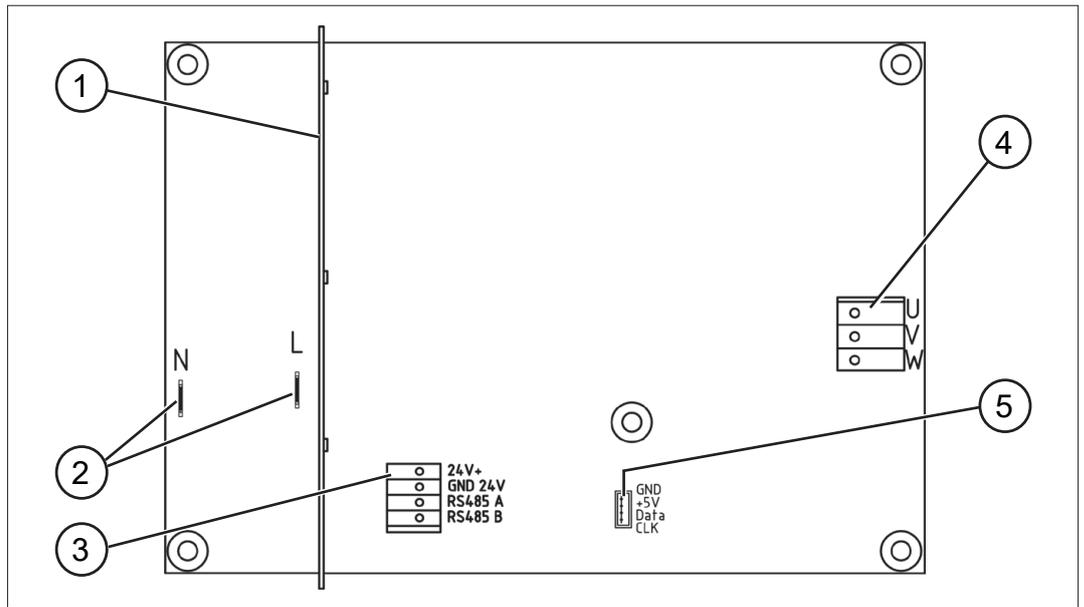

- 1 Shield circuit board
- 2 Power supply connection
- 3 Control cable connection
- 4 Motor connection
- 5 Encoder connection

### 8.1.2 Rating plates

Specifications on the rating plate



- ⇒ In the event of an error, make a note of the type and serial number on the rating plate.
- ⇒ When contacting our Service Department, please provide the type and serial number from the rating plate. This will allow us to provide you with specific support and advice for your device.

#### Vacuum pump rating plate

→ Example Vacuum pump rating plate

The image shows a rectangular rating plate for a vacuum pump. At the top, it features the 'vacuubrand' logo. Below the logo, the text reads 'VACUUM PUMP' and 'VACUU·PURE 10'. To the right of this text is the CE mark. The next line shows 'S/N: 123456789'. Below that is '2020 / 06'. The following two lines are 'max. .... m³/h' and '..... mbar'. The next line is '100-230 V, 50/60 Hz, 700 W'. At the bottom, it says 'VACUUBRAND GMBH+CO KG', 'Alfred - Zippe - Str. 4', '97877 Wertheim', and 'Made in Germany'. There are two warning symbols: a yellow triangle with an exclamation mark on the left and a yellow triangle with three wavy lines on the right. Lines connect the labels on the left to the corresponding information on the plate.

#### Frequency converter rating plate

→ Example Frequency converter rating plate

The image shows a rectangular rating plate for a frequency converter. At the top, it features the 'VACUUBRAND GMBH + CO KG' logo. Below the logo, the text reads 'FC 700S 10' and '2020 / 07'. The next line shows 'SN 123456789'. Below that is '100-230 V, 50/60 Hz'. The following two lines are '700 W' and 'VACUU·BUS®'. At the bottom, it says 'VACUUBRAND GMBH + CO KG', 'Alfred - Zippe - Str. 4', '97877 Wertheim', and 'Made in Germany'. There is a 'vacuubrand' logo at the bottom left. Lines connect the labels on the left to the corresponding information on the plate.

### 8.1.3 Wetted materials

Wetted materials

Component	Wetted materials
Inlet flange, outlet flange, silencer, end cover of the pump unit	PPS
Spindles	PEEK
Stator, bearing plate	Aluminum
Gaskets, flat gasket at the outlet	FKM
Non-return valve	PPS / PTFE / chemically resistant fluoroelastomer
Hose between non-return valve and pump unit	PTFE
Bonding/sealing of the silencer	Epoxy resin adhesive
<b>Optional:</b>	
Silencer	PBT, PVF

## 8.2 Ordering information

Ordering information  
for vacuum pump

<b>Vacuum pump</b>		Order no.
VACUU·PURE 10	CEE	20750000
	CH	20750001
	UK	20750002
	US	20750003
	CN	20750006
	IN	20750007

Ordering information  
for accessories

<b>Accessories</b>	Order no.
VACUU·PURE Shuttle	20751800
Silencer with 90 ° elbow, KF DN 25	20750801
Adapter KF DN 25 / SW DN 15, aluminum	20662519
Elbow KF DN 25/25, aluminum	20669405
Stainless steel hose KF DN 25 (l = 1000 mm)	20673337
Centering and sealing ring KF DN 25 PBT/FKM	20660196
Clamping ring KF DN 25, aluminum	20660001
Hose for outlet, d <sub>i</sub> 19 mm, PVC (by the meter)	20686055
VACUU·SELECT package for fine vacuum control with VACUU·SELECT controller, VACUU·VIEW extended, in-line solenoid valve VV-B 15C, connecting parts KF DN 25, 100 – 230 V / 50 – 60 Hz	20700100
Vacuum gauge VACUU·VIEW extended, 1100 – 0.001 mbar, VACUU·BUS	20683210
In-line solenoid valve VV-B 15C, VACUU·BUS	20674215
VACUU·BUS Y adapter	20636656
Extension cable VACUU·BUS, 0.5 m	20612875
Extension cable VACUU·BUS, 2 m	20612552
Extension cable VACUU·BUS, 5 m	20612931
Extension cable VACUU·BUS, 10 m	22618493
VACUU·BUS Communication Kit, USB to VACUU·BUS converter	20683230

Ordering information  
for spare parts

<b>Spare parts</b>	Order no.
Filter air inlet (regeneration mode)	23126384
Device fuse 8 AT 5x20 (2x)	20612374
O-ring inlet flange	23126349
Flat gasket at outlet (FKM) (2x)	23126456

Power cord	CEE	20612058
	CH	20676021
	CN	20635997
	IN	20635365
	UK	20676020
	US	20612065

### Sources of supply

International  
sales offices and  
distribution

Purchase original accessories and original spare parts from a subsidiary of **VACUUBRAND GMBH + CO KG** or your local distributor.



Information about our complete product range is available in the current [product catalog](#).

⇒ Your local distributor or **VACUUBRAND GMBH + CO KG** [sales office](#) is available to assist you with orders, questions on vacuum control and optimal accessories.

## 8.3 Service

Service offer and  
service range

Take advantage of the comprehensive range of services available from **VACUUBRAND GMBH + CO KG**.



### Services in detail

- Product consultation and practical solutions
- Fast delivery of spare parts and accessories
- Professional maintenance
- Immediate repairs processing
- On-site service (on request)
- With Health and Safety Clearance form: return, disposal

⇒ Visit our website for further information: [www.vacuubrand.com](http://www.vacuubrand.com).

### Service handling

Meet terms of  
service

⇒ Follow these headings: VACUUBRAND > Support > [Service](#)



Reduce downtime, speed up processing. Please have the required data and documents at hand when contacting our Service Department.

- ▶ Your order can be quickly and easily processed.
- ▶ Hazards can be prevented.
- ▶ A brief description and/or photos will help locate the source of the error.

## 8.4 Index

Index	<b>A</b>		
	Abbreviations .....	10	
	Accessories .....	76	
	Action steps .....	9	
	Additional symbols .....	8	
	Advanced operation .....	47	
	Air inlet filter .....	68	
	Autostart .....	21, 46	
	Avoid overpressure .....	19	
	<b>B</b>		
	Blockage protection .....	23	
	<b>C</b>		
	Cleaning and maintenance .....	65	
	Clean the fan grilles .....	67	
	Condensate .....	20	
	Control panel .....	42	
	Copyright © .....	5	
	<b>D</b>		
	Display conventions .....	7	
	Display elements .....	43	
	Display of operating steps .....	9	
	Disposal .....	23	
	Distributors .....	77	
	<b>E</b>		
	EC Declaration of Conformity .....	81	
	Electrical connection .....	41	
	Eliminate sources of danger .....	19	
	Error – Cause – Remedy .....	59	
	Error indication .....	57	
	Error messages .....	56	
	Explanation of safety symbols .....	8	
	<b>F</b>		
	Factory setting .....	49	
	Frequency converter rating plate .....	74	
	<b>G</b>		
	Goods receipt .....	31	
	<b>I</b>		
	Icons .....	8	
	Improper use .....	14	
	In-line solenoid valve .....	53	
	Installation and connection .....	31	
	Instruction .....	9	
	Instruction modules .....	6	
	Intended use .....	13	
	<b>L</b>		
	Labels and signs .....	22	
	Limitation of use .....	33	
	<b>M</b>		
	Maintain minimum distance .....	22	
	Mandatory sign .....	8	
	Manual structure .....	6	
	Minimum distances .....	33	
	Misuse .....	14	
	Modbus RTU protocol .....	30	
	<b>N</b>		
	Non-return valve .....	10	
	<b>O</b>		
	Operating elements .....	43	
	Operating steps as graphics .....	9	
	Operator obligations .....	15	
	Ordering information .....	76	
	Outlet connection (OUT) .....	38	
	Outlet line .....	38	
	Overheating .....	22	
	Overheating protection .....	23	
	<b>P</b>		
	Perform bus scan .....	52	
	Personnel obligations .....	15	
	Personnel qualification .....	16	
	Power cord .....	41	
	Prevent condensate return .....	19, 20	
	Product description .....	24	
	Product-specific terms .....	10	
	Prohibition sign .....	8	
	Protective clothing .....	17	
	<b>Q</b>		
	Qualification description .....	16	
	Quality standard .....	17	
	<b>R</b>		
	Regeneration mode .....	10, 19, 25, 45	
	Remote mode .....	50	
	Replace the device fuse .....	69	
	Residual energy .....	21	
	Responsibility matrix .....	16	
	Restart, automatic .....	21, 46	
	Rotate the inlet flange .....	36	
	<b>S</b>		
	Safety information .....	13	
	Safety precautions .....	17	
	Service handling .....	78	
	Service range .....	78	
	Shutdown .....	54	
	Silencer .....	39	
	Sources of supply .....	77	
	Spare parts .....	76	
	Start .....	44	
	Stop .....	44	
	Switch on .....	42	
	Symbols .....	8	
	<b>T</b>		
	Target groups .....	16	
	Technical data for vacuum pump .....	70	
	Technical information .....	70	
	Technical support .....	58	
	Term definitions .....	10	

Index	<b>U</b>	
	Unpacking .....	31
	User information .....	5
	<b>V</b>	
	VACUU·BUS .....	11
	VACUU·BUS accessories .....	29, 51
	VACUU·BUS address .....	11
	VACUU·BUS client .....	11
	VACUU·BUS configuration .....	11
	VACUU·BUS connector .....	11
	Vacuum connection (IN) .....	34
	Vacuum pump rating plate .....	74
	VACUU·PURE Shuttle .....	27
	VACUU·VIEW (extended) .....	53
	<b>W</b>	
	Warm up times .....	44
	Warm-up times .....	44
	Warnings .....	56
	Warning symbol .....	8
	Wetted materials .....	75

## 8.5 EC Declaration of conformity

**EU Declaration of Conformity**  
**EC Declaration of Conformity**  
**Déclaration CE de conformité**



Hersteller / Manufacturer / Fabricant:

**VACUUBRAND GMBH + CO KG** · Alfred-Zippe-Str. 4 · 97877 Wertheim · Germany

Hiermit erklärt der Hersteller, dass das Produkt konform ist mit den Bestimmungen der Richtlinien:

Hereby the manufacturer declares that the device is in conformity with the directives:

Par la présente, le fabricant déclare, que le dispositif est conforme aux directives:

2006/42/EG (M-RL), 2014/30/EU (EMV-RL),  
 2011/65/EU, 2015/863 (RoHS-2)

Vakuumpumpe / Vacuum pump / Pompe à vide

Typ / Type / Type: **VACUU·PURE 10**

Artikelnummer / Order number / Numéro d'article: **20750005**

Seriennummer / Serial number / Numéro de série: Siehe Typenschild / See rating plate / Voir plaque signalétique

Angewandte harmonisierte Normen / Harmonized standards applied / Normes harmonisées utilisées: DIN EN ISO 12100:2011, DIN EN 1012-2:2011, IEC 61010-1:2010 (Ed. 3), DIN EN 61010-1:2011, DIN EN 61326-1:2013, DIN EN IEC 63000:2019

Bevollmächtigter für die Zusammenstellung der technischen Unterlagen / Person authorised to compile the technical file / Personne autorisée à constituer le dossier technique: Dr. F. Gitmans · VACUUBRAND GMBH + CO KG · Germany

Ort, Datum / place, date / lieu, date: Wertheim, 16.07.2020

(Dr. F. Gitmans)

*Geschäftsführer / Managing Director /  
 Gérant*

i. A.

(Dr. A. Wollschläger)

*Regulatory Affairs Manager*

**VACUUBRAND GMBH + CO KG**

Alfred-Zippe-Str. 4  
 97877 Wertheim

Phone: +49 9342 808-0

Fax: +49 9342 808-5555

E-Mail: [info@vacuubrand.com](mailto:info@vacuubrand.com)

Web: [www.vacuubrand.com](http://www.vacuubrand.com)

## DECLARATION OF CONFORMITY – China RoHS 2

VACUUBRAND GMBH + CO KG has made reasonable efforts to ensure that hazardous materials and substances may not be used in its products.

In order to determine the concentration of hazardous substances in all homogeneous materials of the subassemblies, a “Product Conformity Assessment” (PCA) procedure was performed. As defined in GB/T 26572 the “Maximum Concentration Value” limits (MCV) apply to these restricted substances:

- Lead (Pb): 0.1%
- Mercury (Hg): 0.1%
- Cadmium (Cd): 0.01%
- Hexavalent chromium (Cr(+VI)): 0.1%
- Polybrominated biphenyls (PBB): 0.1%
- Polybrominated diphenyl ether (PBDE): 0.1%

### Environmentally Friendly Use Period (EFUP)

EFUP defines the period in years during which the hazardous substances contained in electrical and electronic products will not leak or mutate under normal operating conditions. During normal use by the user such electrical and electronic products will not result in serious environmental pollution, cause serious bodily injury or damage to the user's assets.

The Environmentally Friendly Use Period for VACUUBRAND products is 40 years.



此表格是按照SJ/T 11364-2014中规定所制定的。  
This table is created according to SJ/T 11364-2014.

MATERIAL CONTENT DECLARATION FOR VACUUBRAND PRODUCTS							
部件名称 Part name	有毒有害物质或元素 Hazardous substances						环保期限标识 EFUP
	铅 Pb	汞 Hg	镉 Cd	六价铬 Cr(+VI)	多溴联苯 PBB	多溴二苯醚 PBDE	
包装 Packaging	○	○	○	○	○	○	
塑料外壳 / 组件 Plastic housing / parts	○	○	○	○	○	○	
真空油 Vacuum oil	○	○	○	○	○	○	
电池 Battery	○	○	○	○	○	○	
玻璃 Glass	X	○	○	○	○	○	
电子电气组件 Electrical and electronic parts	X	○	○	○	○	○	
控制器 / 测量设备 Controller / measuring device	X	○	○	○	○	○	
金属外壳 / 组件 Metal housing / parts	X	○	○	○	○	○	
电机 Motor	X	○	○	○	○	○	
配件 Accessories	X	○	○	○	○	○	

**注释:** 此表格适用于所有产品。以上列出的元件或组件不一定都属于所附产品的组成。

**Note:** Table applies to all products. Some of the components or parts listed above may not be part of the enclosed product.

- O: 表示该有毒有害物质在该部件所有均质材料中的含量均在GB/T 26572规定的限量要求以下。  
O: Indicates that the above mentioned hazardous substance contained in all homogeneous materials of the part is below the required limit as defined in GB/T 26572.
- X: 表示该有毒有害物质至少在该部件某一均质材料中的含量超出GB/T 26572规定的限量要求。  
X: Indicates that the above mentioned hazardous substance contained in at least one of the homogeneous materials of this part is above the required limit as defined in GB/T 26572.

除上表所示信息外，还需声明的是，这些部件并非是有意图用铅（Pb）、汞（Hg）、铬（Cd）、六价铬（Cr(+VI)）、多溴联苯（PBB）或多溴二苯醚（PBDE）来制造的。

Apart from the disclosures in the above table, the subassemblies are not intentionally manufactured or formulated with lead (Pb), mercury (Hg), cadmium (Cd), hexavalent chromium (Cr+VI), polybrominated biphenyls (PBB), and polybrominated diphenyl ethers (PBDE).

Products manufactured by VACUUBRAND may enter into further devices (e.g., rotary evaporator) or can be used together with other appliances (e.g., usage as booster pumps).

With these products and appliances in particular, please note the EFUP labeled on these products. VACUUBRAND will not take responsibility for the EFUP of those products and appliances.

Place, date: Wertheim, 06/04/2020



(Dr. F. Gitmans)  
Managing Director



i.A. (Dr. A. Wollschläger)  
Regulatory Affairs Manager

**VACUUBRAND GMBH + CO KG**  
Alfred-Zippe-Str. 4  
97877 Wertheim  
Germany

Tel.: +49 9342 808-0  
Fax: +49 9342 808-5555  
E-Mail: [info@vacuubrand.com](mailto:info@vacuubrand.com)  
Web: [www.vacuubrand.com](http://www.vacuubrand.com)











Technology for Vacuum Systems

Manufacturer:

**VACUUBRAND GMBH + CO KG**  
**Alfred-Zippe-Str. 4**  
**97877 Wertheim**  
**GERMANY**

Phone:

Head office +49 9342 808-0

Sales +49 9342 808-5550

Service +49 9342 808-5660

Fax: +49 9342 808-5555

Email: [info@vacuubrand.com](mailto:info@vacuubrand.com)

Web: [www.vacuubrand.com](http://www.vacuubrand.com)